
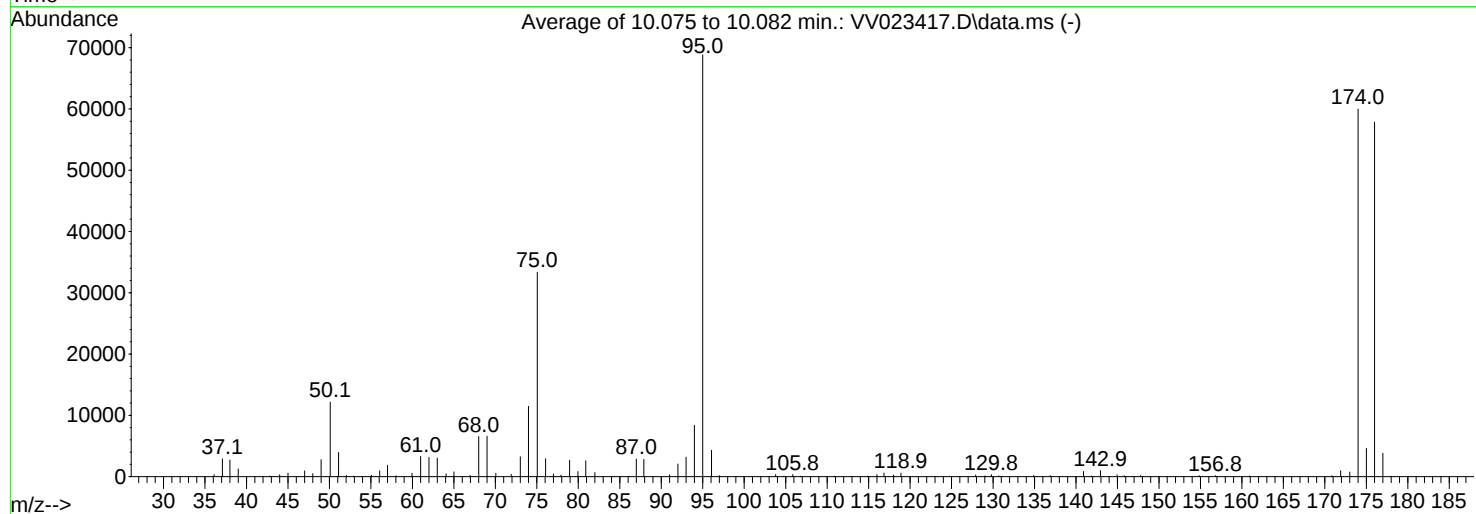


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111221\
 Data File : VV023417.D
 Acq On : 12 Nov 2021 03:23
 Operator : SY/MD
 Sample : BFB233
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB233

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 17 02:49:39 2021

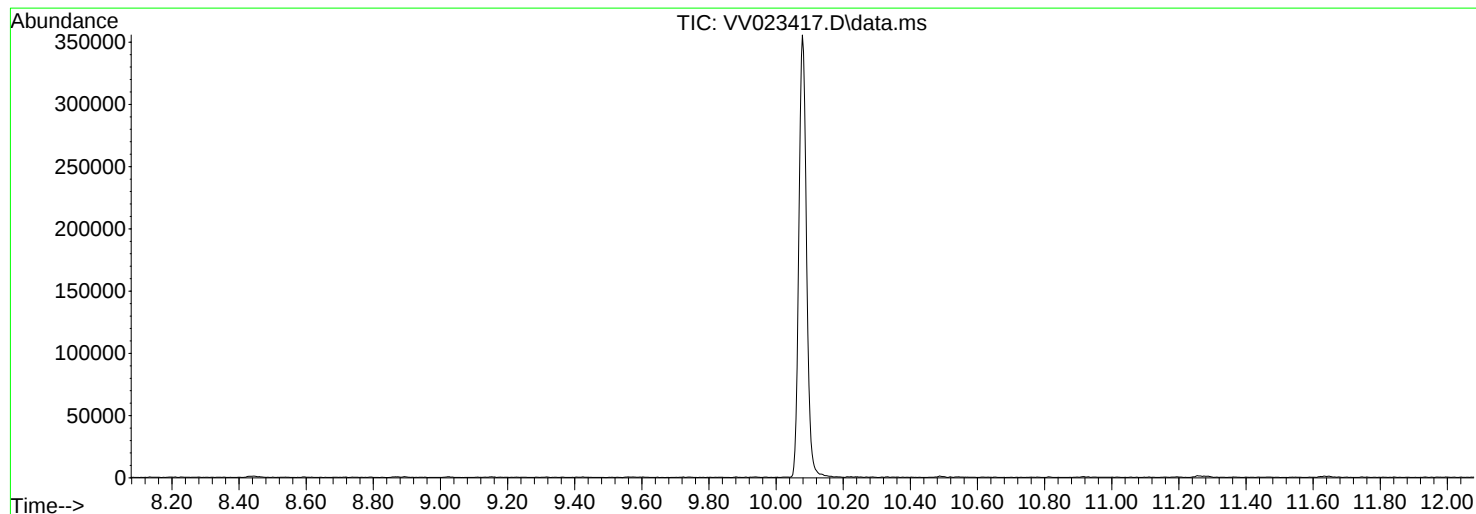

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12163	PASS
75	95	30	80	48.4	33344	PASS
95	95	100	100	100.0	68832	PASS
96	95	5	9	6.3	4305	PASS
173	174	0.00	2	1.3	771	PASS
174	95	50	120	87.1	59971	PASS
175	174	5	9	7.7	4609	PASS
176	174	95	105	96.5	57864	PASS
177	176	5	10	6.6	3814	PASS

m/z	Abundance
36.20	140.0
40.00	176.0
44.10	326.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.10	537.0
37.10	2861.0
38.00	2828.0
39.00	1325.0
40.00	182.0
42.80	107.0
44.00	624.0
45.00	563.0
46.30	105.0
47.00	932.0
48.00	522.0
49.00	2836.0
50.10	12359.0
51.10	3769.0
52.00	169.0
53.00	106.0
55.00	251.0
56.10	961.0
57.00	1775.0
58.00	110.0
60.00	586.0
61.00	3219.0
62.00	3078.0
63.00	2993.0
64.00	475.0
65.00	804.0
67.00	205.0
68.00	6655.0
69.00	6879.0
70.00	596.0
71.90	384.0
73.00	3225.0
74.00	11463.0
75.10	32936.0
76.00	3062.0
77.00	425.0
77.90	286.0
78.90	2684.0
79.90	791.0
80.90	2472.0
82.00	678.0
87.00	2892.0
87.90	2873.0
91.00	308.0
92.00	1977.0
93.00	3001.0
94.00	8112.0
95.00	67600.0
96.10	4278.0
97.00	168.0
103.80	321.0
104.80	107.0
105.90	325.0
106.80	133.0
111.00	109.0
116.00	332.0
116.80	559.0
117.90	264.0
118.90	552.0
127.90	271.0
129.10	106.0
129.80	323.0
130.70	112.0
131.10	119.0
134.90	173.0
136.90	194.0
140.90	791.0
141.90	112.0
142.90	1006.0
145.00	270.0
145.80	174.0
147.80	182.0
154.80	143.0
156.90	157.0
160.90	102.0
170.80	170.0
171.90	906.0
173.00	704.0
174.00	57664.0
175.00	4626.0
176.00	55184.0
177.00	3683.0
177.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.10	508.0
37.10	2975.0
38.00	2821.0
39.00	1321.0
40.00	205.0
42.90	119.0
43.90	649.0
45.00	575.0
47.00	991.0
48.00	531.0
49.00	2890.0
50.10	12550.0
51.10	4080.0
52.10	183.0
53.00	114.0
55.00	231.0
56.10	984.0
57.00	1922.0
58.00	123.0
60.00	591.0
61.00	3417.0
62.00	3227.0
63.00	3152.0
64.10	461.0
65.00	814.0
66.20	100.0
66.90	208.0
68.00	6757.0
69.00	6748.0
70.00	540.0
71.90	392.0
73.00	3387.0
74.00	11900.0
75.10	34296.0
76.00	2963.0
77.00	471.0
77.90	246.0
79.00	2748.0
79.90	873.0
80.90	2671.0
82.00	692.0
87.00	2983.0
87.90	2902.0
91.00	328.0
92.00	2130.0
93.00	3339.0
94.00	8636.0
95.00	71040.0
96.10	4389.0
97.00	182.0
103.80	346.0
104.80	114.0
105.90	353.0
106.80	107.0
114.90	106.0
116.00	356.0
116.90	593.0
118.00	279.0
118.90	607.0
127.90	276.0
129.10	134.0
129.80	363.0
130.70	140.0
134.90	193.0
136.90	196.0
140.90	873.0
141.90	122.0
143.00	997.0
144.90	317.0
145.80	171.0
147.80	177.0
154.90	161.0
156.80	186.0
160.90	128.0
170.80	160.0
171.90	967.0
172.90	797.0
174.00	61792.0
175.00	4730.0
176.00	59608.0
177.00	3936.0
178.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233

m/z	Abundance
36.10	434.0
37.10	2866.0
38.00	2539.0
39.00	1128.0
40.10	224.0
42.90	102.0
43.90	661.0
45.00	571.0
47.00	941.0
48.00	481.0
49.00	2591.0
50.10	11581.0
51.10	3963.0
52.10	173.0
52.90	121.0
53.90	102.0
55.10	228.0
56.00	870.0
57.00	1868.0
58.10	126.0
59.90	570.0
61.00	3225.0
62.00	3109.0
63.00	2915.0
64.10	447.0
65.00	737.0
66.90	191.0
68.00	6256.0
69.00	6216.0
70.10	483.0
71.90	377.0
73.00	3103.0
74.00	11018.0
75.00	32800.0
76.10	2782.0
77.00	461.0
77.90	251.0
79.00	2606.0
80.00	863.0
80.90	2628.0
82.00	663.0
82.90	105.0
86.20	119.0
87.00	2671.0
87.90	2728.0
91.00	321.0
92.00	2077.0
93.00	3253.0
94.00	8377.0
95.00	67856.0
96.00	4249.0
97.00	157.0
103.80	340.0
105.80	345.0
110.80	110.0
112.80	106.0
114.90	116.0
116.00	308.0
116.90	581.0
118.10	272.0
118.90	586.0
127.90	256.0
129.00	160.0
129.80	324.0
130.70	148.0
134.90	170.0
136.90	186.0
140.90	919.0
141.80	106.0
143.00	968.0
143.90	119.0
144.90	347.0
145.80	150.0
146.70	106.0
147.80	164.0
154.90	201.0
156.70	194.0
161.00	136.0
170.90	147.0
171.90	995.0
173.10	813.0
174.00	60456.0
175.00	4470.0
176.00	58800.0
177.00	3824.0

Instrument :
MSVOA_V
ClientSampleId :
BFB233