
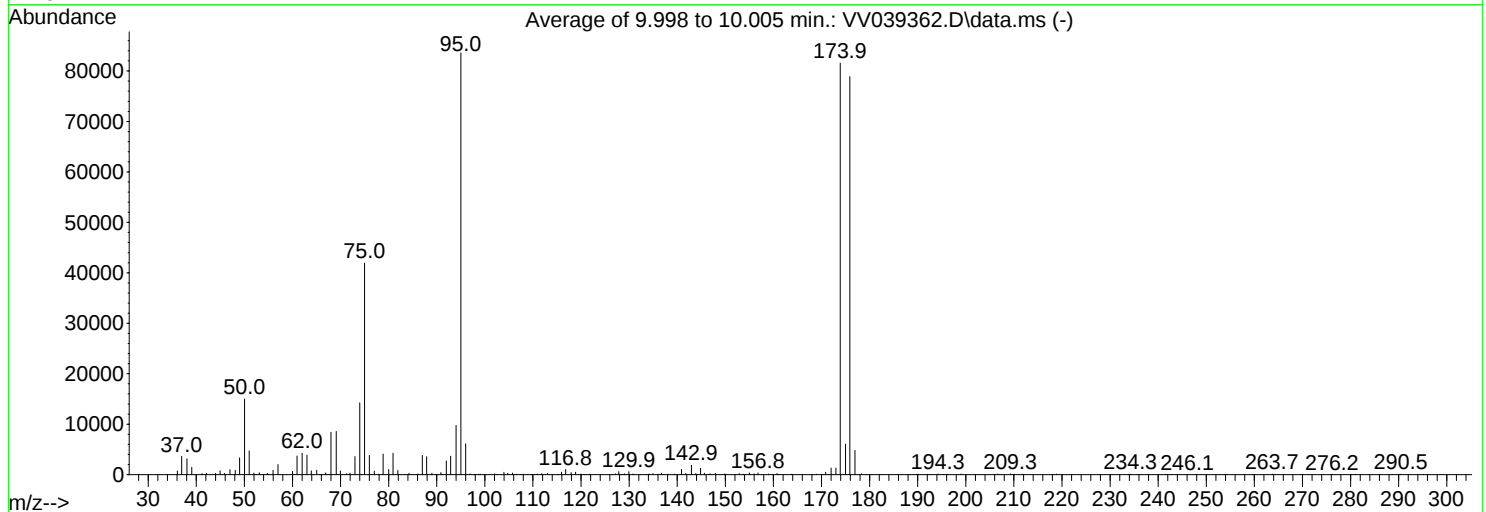


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111225\
Data File : VV039362.D
Acq On : 12 Nov 2025 08:09
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V111125W.M
Title : SW846 8260
Last Update : Wed Nov 12 01:49:22 2025

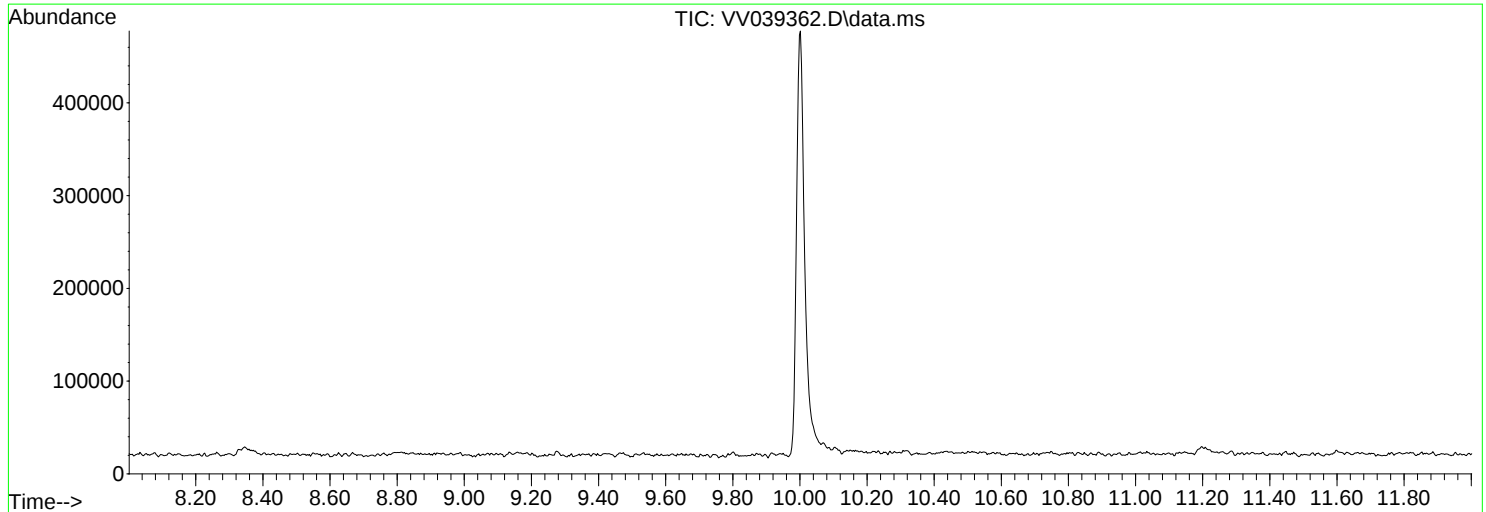

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	15012	PASS
75	95	30	60	50.2	41936	PASS
95	95	100	100	100.0	83600	PASS
96	95	5	9	7.3	6111	PASS
173	174	0.00	2	1.6	1303	PASS
174	95	50	100	97.6	81568	PASS
175	174	5	9	7.4	6055	PASS
176	174	95	101	96.7	78893	PASS
177	176	5	9	6.1	4836	PASS