


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111319\
 Data File : VV013596.D
 Acq On : 13 Nov 2019 08:29
 Operator : SY/MD
 Sample : BFB60
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB60

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Nov 14 06:01:41 2019

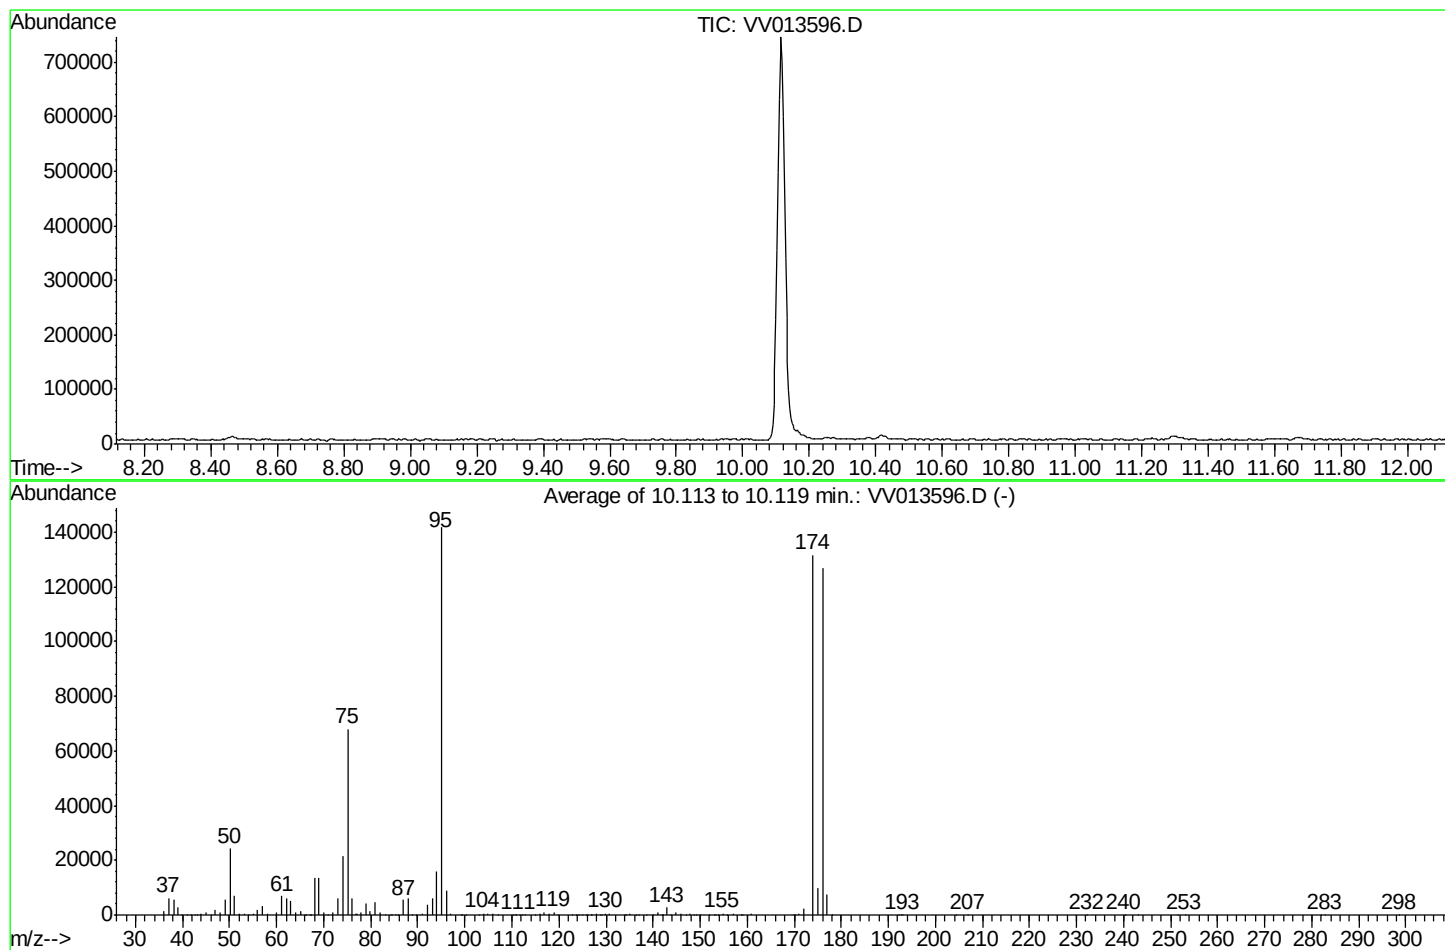

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	24291	PASS
75	95	30	80	48.0	68055	PASS
95	95	100	100	100.0	141717	PASS
96	95	5	9	6.2	8792	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.9	131693	PASS
175	174	5	9	7.5	9938	PASS
176	174	95	101	96.4	126968	PASS
177	176	5	9	6.1	7712	PASS

m/z	Abundance
36.10	1358.0
37.10	6417.0
38.10	6038.0
39.10	2881.0
40.00	1040.0
40.90	339.0
41.80	153.0
42.70	194.0
43.20	309.0
44.00	1448.0
45.10	1114.0
45.90	243.0
46.90	1928.0
47.90	1018.0
49.00	6097.0
50.00	24664.0
51.10	7098.0
52.10	514.0
53.10	308.0
53.90	272.0
55.00	487.0
56.00	2151.0
57.00	3164.0
58.10	300.0
60.00	1184.0
61.00	7075.0
62.10	6396.0
63.00	5429.0
64.00	1108.0
65.10	1736.0
66.00	219.0
67.00	460.0
68.00	13339.0
69.00	13637.0
70.00	1224.0
70.90	210.0
71.90	792.0
73.00	6280.0
74.00	21608.0
75.10	68184.0
76.10	6203.0
76.90	840.0
77.90	797.0
78.90	4413.0
79.90	1254.0
80.90	4744.0
81.90	924.0
83.10	125.0
84.20	109.0
85.80	200.0
87.00	5940.0
88.00	6334.0
91.00	523.0
92.00	3686.0
93.00	5879.0
94.00	16098.0
95.00	140736.0
96.00	9405.0
97.00	356.0
99.20	102.0
100.30	126.0
103.00	130.0
103.90	622.0
104.80	255.0
105.90	567.0
107.10	193.0
110.70	149.0
111.60	139.0
112.20	192.0
112.80	221.0
114.90	155.0
115.90	604.0
116.80	912.0
118.00	594.0
118.80	983.0
119.70	186.0
122.70	122.0
123.70	114.0
124.10	112.0
124.90	149.0
126.00	141.0
126.80	137.0
127.90	561.0
129.10	282.0
129.90	627.0
130.80	258.0
134.30	121.0
135.00	297.0
136.80	209.0
138.70	107.0
139.80	137.0
140.90	1049.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

141.90	173.0
143.00	2741.0
143.80	249.0
145.00	1259.0
145.80	409.0
147.10	165.0
147.90	431.0
149.20	104.0
149.70	154.0
151.80	131.0
152.90	128.0
153.80	140.0
155.00	400.0
155.70	127.0
157.00	359.0
158.70	228.0
159.00	257.0
160.90	290.0
169.80	131.0
170.90	636.0
171.90	2000.0
174.00	130392.0
175.00	9783.0
176.00	124448.0
176.90	7539.0
177.90	171.0
192.00	113.0
192.70	127.0
193.00	117.0
207.00	106.0
232.30	115.0
298.60	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.00	1378.0
37.10	6490.0
38.10	6032.0
39.10	2968.0
39.90	1138.0
41.00	403.0
41.80	138.0
43.10	265.0
44.00	1449.0
45.10	1124.0
45.90	240.0
46.90	2017.0
47.90	1047.0
49.00	5978.0
50.00	25120.0
51.10	7441.0
52.00	559.0
53.10	258.0
53.80	209.0
55.00	393.0
56.00	2088.0
57.00	3215.0
58.10	360.0
60.00	1330.0
61.10	7185.0
62.00	6102.0
63.00	5599.0
64.00	1067.0
65.10	1687.0
65.90	184.0
66.30	179.0
67.20	432.0
68.00	13850.0
69.00	13764.0
70.00	1349.0
70.90	202.0
71.90	789.0
73.00	6508.0
74.00	22112.0
75.10	70856.0
76.10	6192.0
76.90	791.0
77.90	770.0
79.00	4606.0
79.90	1397.0
80.90	4817.0
81.90	909.0
83.10	120.0
84.20	125.0
84.40	106.0
85.90	205.0
87.00	5765.0
88.00	6337.0
91.00	464.0
92.00	4013.0
93.00	6088.0
94.00	16165.0
95.00	146688.0
96.00	9011.0
97.10	350.0
99.10	129.0
103.00	125.0
103.90	711.0
104.80	305.0
105.90	585.0
107.10	175.0
110.30	123.0
110.70	150.0
111.60	120.0
112.20	176.0
112.80	158.0
114.90	205.0
116.00	657.0
116.80	951.0
117.90	591.0
118.80	1052.0
122.70	121.0
123.70	172.0
124.20	147.0
125.00	116.0
126.00	122.0
126.80	139.0
127.90	463.0
129.10	276.0
129.90	674.0
130.70	309.0
133.90	101.0
135.10	299.0
136.90	235.0
138.70	167.0
139.80	171.0
140.90	1072.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

142.90	2781.0
144.90	1192.0
145.90	396.0
147.00	183.0
147.90	317.0
148.70	170.0
149.20	101.0
150.00	199.0
151.80	200.0
153.00	132.0
153.90	112.0
154.80	466.0
155.70	109.0
157.00	385.0
158.70	203.0
159.10	189.0
161.00	320.0
169.80	135.0
170.80	548.0
171.90	2223.0
174.00	135808.0
175.00	10431.0
176.00	131072.0
176.90	7878.0
178.00	220.0
192.10	116.0
193.00	123.0
207.00	113.0
232.20	105.0
240.20	126.0
243.00	123.0
251.40	111.0
253.00	119.0
298.60	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	1324.0
37.10	5753.0
38.10	5642.0
39.10	2695.0
39.90	1111.0
41.00	364.0
42.60	167.0
43.00	234.0
44.00	1293.0
45.10	1159.0
46.00	257.0
46.90	1806.0
47.90	1021.0
49.10	5408.0
50.10	23528.0
51.10	7255.0
52.00	585.0
53.10	220.0
53.80	196.0
54.90	347.0
56.00	1869.0
57.00	3101.0
58.10	311.0
60.00	1354.0
61.10	6723.0
62.00	5621.0
63.00	5460.0
64.00	954.0
65.00	1544.0
65.90	174.0
66.20	180.0
68.00	13023.0
69.10	12845.0
70.00	1367.0
70.90	151.0
71.90	685.0
73.00	5767.0
74.00	20784.0
75.10	65480.0
76.10	5623.0
77.10	809.0
77.80	609.0
79.00	4247.0
79.90	1390.0
80.90	4445.0
81.90	901.0
84.50	113.0
85.20	111.0
85.80	251.0
87.00	5039.0
88.00	5885.0
88.90	162.0
89.70	103.0
91.00	401.0
92.00	3896.0
93.00	5710.0
94.00	14924.0
95.00	137728.0
96.00	7960.0
97.10	327.0
99.10	113.0
99.40	105.0
102.90	119.0
103.90	727.0
104.90	324.0
106.00	575.0
107.10	139.0
110.90	139.0
111.60	117.0
112.20	131.0
114.90	239.0
116.00	607.0
116.80	919.0
117.90	554.0
118.90	923.0
123.70	187.0
124.10	128.0
125.00	137.0
125.70	136.0
127.00	165.0
127.90	409.0
128.80	347.0
129.90	673.0
130.70	332.0
135.10	237.0
136.50	182.0
137.00	224.0
138.70	173.0
139.90	182.0
140.90	1096.0
142.10	258.0
142.90	2670.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

143.80	229.0
144.90	1065.0
145.80	330.0
146.90	171.0
147.90	300.0
148.70	218.0
150.00	253.0
151.80	223.0
152.80	154.0
153.20	155.0
154.00	162.0
154.80	571.0
157.10	389.0
158.60	157.0
159.20	120.0
161.00	279.0
170.20	143.0
170.80	461.0
171.90	2168.0
174.00	128880.0
175.00	9601.0
176.00	125384.0
176.90	7721.0
178.00	288.0
193.00	101.0
204.30	114.0
206.90	143.0
240.20	106.0
253.00	127.0
281.80	102.0
282.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.20	192.0
35.90	150.0
38.10	118.0
39.10	120.0
40.00	902.0
40.90	139.0
41.30	133.0
42.40	124.0
43.00	170.0
44.00	737.0
45.40	123.0
46.00	161.0
47.60	150.0
48.30	205.0
50.20	146.0
51.80	114.0
52.40	148.0
54.00	166.0
59.30	141.0
60.20	115.0
62.20	118.0
63.20	148.0
69.80	121.0
70.10	105.0
73.10	114.0
75.20	118.0
75.70	103.0
76.90	122.0
81.10	103.0
83.90	105.0
101.80	120.0
115.00	123.0
116.00	116.0
149.70	102.0
163.70	102.0
165.60	106.0
183.30	115.0
187.10	128.0
195.50	149.0
201.20	126.0
228.80	110.0
254.40	127.0
288.00	141.0
295.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60