

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111320\
 Data File : VV019375.D
 Acq On : 13 Nov 2020 14:08
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	108325	108992	14.25%	1.801%
2	1.576	144	151	164	rBV	96974	110951	14.50%	1.833%
3	2.119	309	320	347	rBV	203014	304907	39.86%	5.038%
4	2.306	371	378	384	rBV2	436	720	0.09%	0.012%
5	2.370	396	398	402	rBV	162	173	0.02%	0.003%
6	2.454	420	424	427	rBV2	265	269	0.04%	0.004%
7	2.521	440	445	452	rBV3	779	1091	0.14%	0.018%
8	2.605	468	471	474	rBV2	151	114	0.01%	0.002%
9	2.685	490	496	498	rBV2	193	171	0.02%	0.003%
10	2.711	501	504	509	rVB	183	115	0.02%	0.002%
11	3.058	609	612	614	rBV	134	119	0.02%	0.002%
12	3.068	614	615	619	rVB	232	138	0.02%	0.002%
13	3.106	624	627	630	rBV2	256	224	0.03%	0.004%
14	3.193	652	654	657	rBV	175	140	0.02%	0.002%
15	3.277	677	680	683	rBV	153	148	0.02%	0.002%
16	3.296	685	686	690	rBB	208	130	0.02%	0.002%
17	3.389	711	715	718	rBB	266	191	0.02%	0.003%
18	3.405	718	720	723	rBB2	249	141	0.02%	0.002%
19	3.444	729	732	738	rBV	296	275	0.04%	0.005%
20	3.492	744	747	750	rVB2	287	210	0.03%	0.003%
21	3.547	759	764	767	rBB	148	151	0.02%	0.002%
22	3.576	770	773	775	rBV	133	118	0.02%	0.002%
23	3.682	805	806	809	rBV	230	122	0.02%	0.002%
24	3.769	830	833	839	rBB2	256	227	0.03%	0.004%
25	3.907	866	876	912	rBV	45062	143652	18.78%	2.374%
26	4.370	1003	1020	1043	rVV	131118	323528	42.29%	5.346%
27	4.534	1067	1071	1073	rBV3	272	215	0.03%	0.004%
28	4.569	1078	1082	1086	rBB2	314	296	0.04%	0.005%
29	4.605	1090	1093	1096	rBV2	301	316	0.04%	0.005%
30	4.656	1105	1109	1112	rBV	190	207	0.03%	0.003%
31	4.753	1137	1139	1142	rBV	167	132	0.02%	0.002%
32	4.788	1148	1150	1152	rBV	250	160	0.02%	0.003%
33	4.913	1187	1189	1194	rBV	150	178	0.02%	0.003%
34	4.968	1204	1206	1210	rVB2	254	195	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111320\
 Data File : VV019375.D
 Acq On : 13 Nov 2020 14:08
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

35	5.064	1219	1236	1258	rBV2	297128	764980	100.00%	12.641%
36	5.235	1287	1289	1292	rVB2	212	139	0.02%	0.002%
37	5.264	1292	1298	1301	rBV3	366	436	0.06%	0.007%
38	5.302	1307	1310	1311	rBV	262	153	0.02%	0.003%
39	5.335	1317	1320	1323	rBV2	290	198	0.03%	0.003%
40	5.399	1339	1340	1344	rVB	255	135	0.02%	0.002%
41	5.418	1344	1346	1349	rBV	127	115	0.02%	0.002%
42	5.450	1354	1356	1363	rVB2	249	281	0.04%	0.005%
43	5.498	1368	1371	1374	rBV	161	158	0.02%	0.003%
44	5.547	1383	1386	1387	rBV	256	152	0.02%	0.003%
45	5.589	1395	1399	1401	rBV	222	200	0.03%	0.003%
46	5.637	1401	1414	1442	rVV	246229	489370	63.97%	8.087%
47	5.923	1492	1503	1517	rBV	19129	37651	4.92%	0.622%
48	6.023	1532	1534	1538	rVB2	253	128	0.02%	0.002%
49	6.087	1541	1554	1574	rBV	168119	340728	44.54%	5.630%
50	6.174	1579	1581	1583	rBV2	445	201	0.03%	0.003%
51	6.222	1593	1596	1600	rBV3	364	300	0.04%	0.005%
52	6.306	1619	1622	1624	rBV3	264	175	0.02%	0.003%
53	6.351	1631	1636	1640	rBB	189	221	0.03%	0.004%
54	6.373	1640	1643	1647	rBV	225	235	0.03%	0.004%
55	6.437	1659	1663	1665	rBV	167	129	0.02%	0.002%
56	6.450	1665	1667	1669	rVV2	258	166	0.02%	0.003%
57	6.473	1673	1674	1677	rVV	253	146	0.02%	0.002%
58	6.495	1678	1681	1684	rVB	297	202	0.03%	0.003%
59	6.537	1692	1694	1698	rBB	237	170	0.02%	0.003%
60	6.560	1698	1701	1703	rBB2	233	130	0.02%	0.002%
61	6.579	1703	1707	1711	rBB	169	194	0.03%	0.003%
62	6.637	1722	1725	1727	rBV	132	114	0.01%	0.002%
63	6.781	1766	1770	1775	rVB	294	332	0.04%	0.005%
64	6.820	1780	1782	1784	rVV	252	141	0.02%	0.002%
65	6.881	1798	1801	1803	rBV	201	153	0.02%	0.003%
66	7.003	1828	1839	1865	rBV	98949	178677	23.36%	2.953%
67	7.135	1876	1880	1883	rBV3	357	241	0.03%	0.004%
68	7.187	1892	1896	1901	rBV2	157	197	0.03%	0.003%
69	7.232	1908	1910	1913	rBV	212	114	0.01%	0.002%
70	7.248	1913	1915	1919	rVB	278	130	0.02%	0.002%
71	7.334	1929	1942	1967	rBV	357739	614051	80.27%	10.147%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111320\
 Data File : VV019375.D
 Acq On : 13 Nov 2020 14:08
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis

72	7.640	2026	2037	2055	rBV2	74629	127522	16.67%	2.107%
73	7.846	2097	2101	2102	rBV	199	139	0.02%	0.002%
74	8.006	2145	2151	2154	rBV3	563	491	0.06%	0.008%
75	8.106	2172	2182	2213	rBV2	155589	300746	39.31%	4.970%
76	8.633	2343	2346	2348	rBV	174	133	0.02%	0.002%
77	8.666	2352	2356	2358	rBV	139	141	0.02%	0.002%
78	8.756	2380	2384	2385	rBV	146	124	0.02%	0.002%
79	8.871	2405	2420	2438	rBV	380602	620770	81.15%	10.258%
80	9.206	2521	2524	2526	rBV	177	147	0.02%	0.002%
81	9.830	2713	2718	2721	rBV2	186	226	0.03%	0.004%
82	9.897	2735	2739	2742	rBV2	166	122	0.02%	0.002%
83	9.984	2763	2766	2773	rVB2	227	205	0.03%	0.003%
84	10.235	2832	2844	2865	rVB	212637	332487	43.46%	5.494%
85	10.309	2865	2867	2871	rVB2	176	118	0.02%	0.002%
86	10.434	2904	2906	2909	rBV	235	153	0.02%	0.003%
87	10.714	2989	2993	2995	rBV	209	174	0.02%	0.003%
88	10.775	3007	3012	3015	rBV2	259	282	0.04%	0.005%
89	11.042	3091	3095	3098	rBV	227	237	0.03%	0.004%
90	11.267	3154	3165	3185	rBV	398326	616368	80.57%	10.185%
91	11.643	3271	3282	3299	rBV	398542	619248	80.95%	10.233%
92	11.891	3354	3359	3362	rBV2	227	279	0.04%	0.005%
93	12.247	3466	3470	3475	rVB2	243	315	0.04%	0.005%
94	12.929	3679	3682	3684	rBV	394	258	0.03%	0.004%
95	13.157	3750	3753	3755	rBV2	282	133	0.02%	0.002%
96	13.440	3838	3841	3848	rBV	193	149	0.02%	0.002%
97	13.691	3917	3919	3921	rBV	298	127	0.02%	0.002%
98	14.080	4037	4040	4042	rBV	377	207	0.03%	0.003%
99	14.189	4072	4074	4077	rBV2	292	185	0.02%	0.003%
100	14.546	4183	4185	4187	rBV	366	152	0.02%	0.003%


Sum of corrected areas: 6051597

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111320\
Data File : VV019375.D
Acq On : 13 Nov 2020 14:08
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

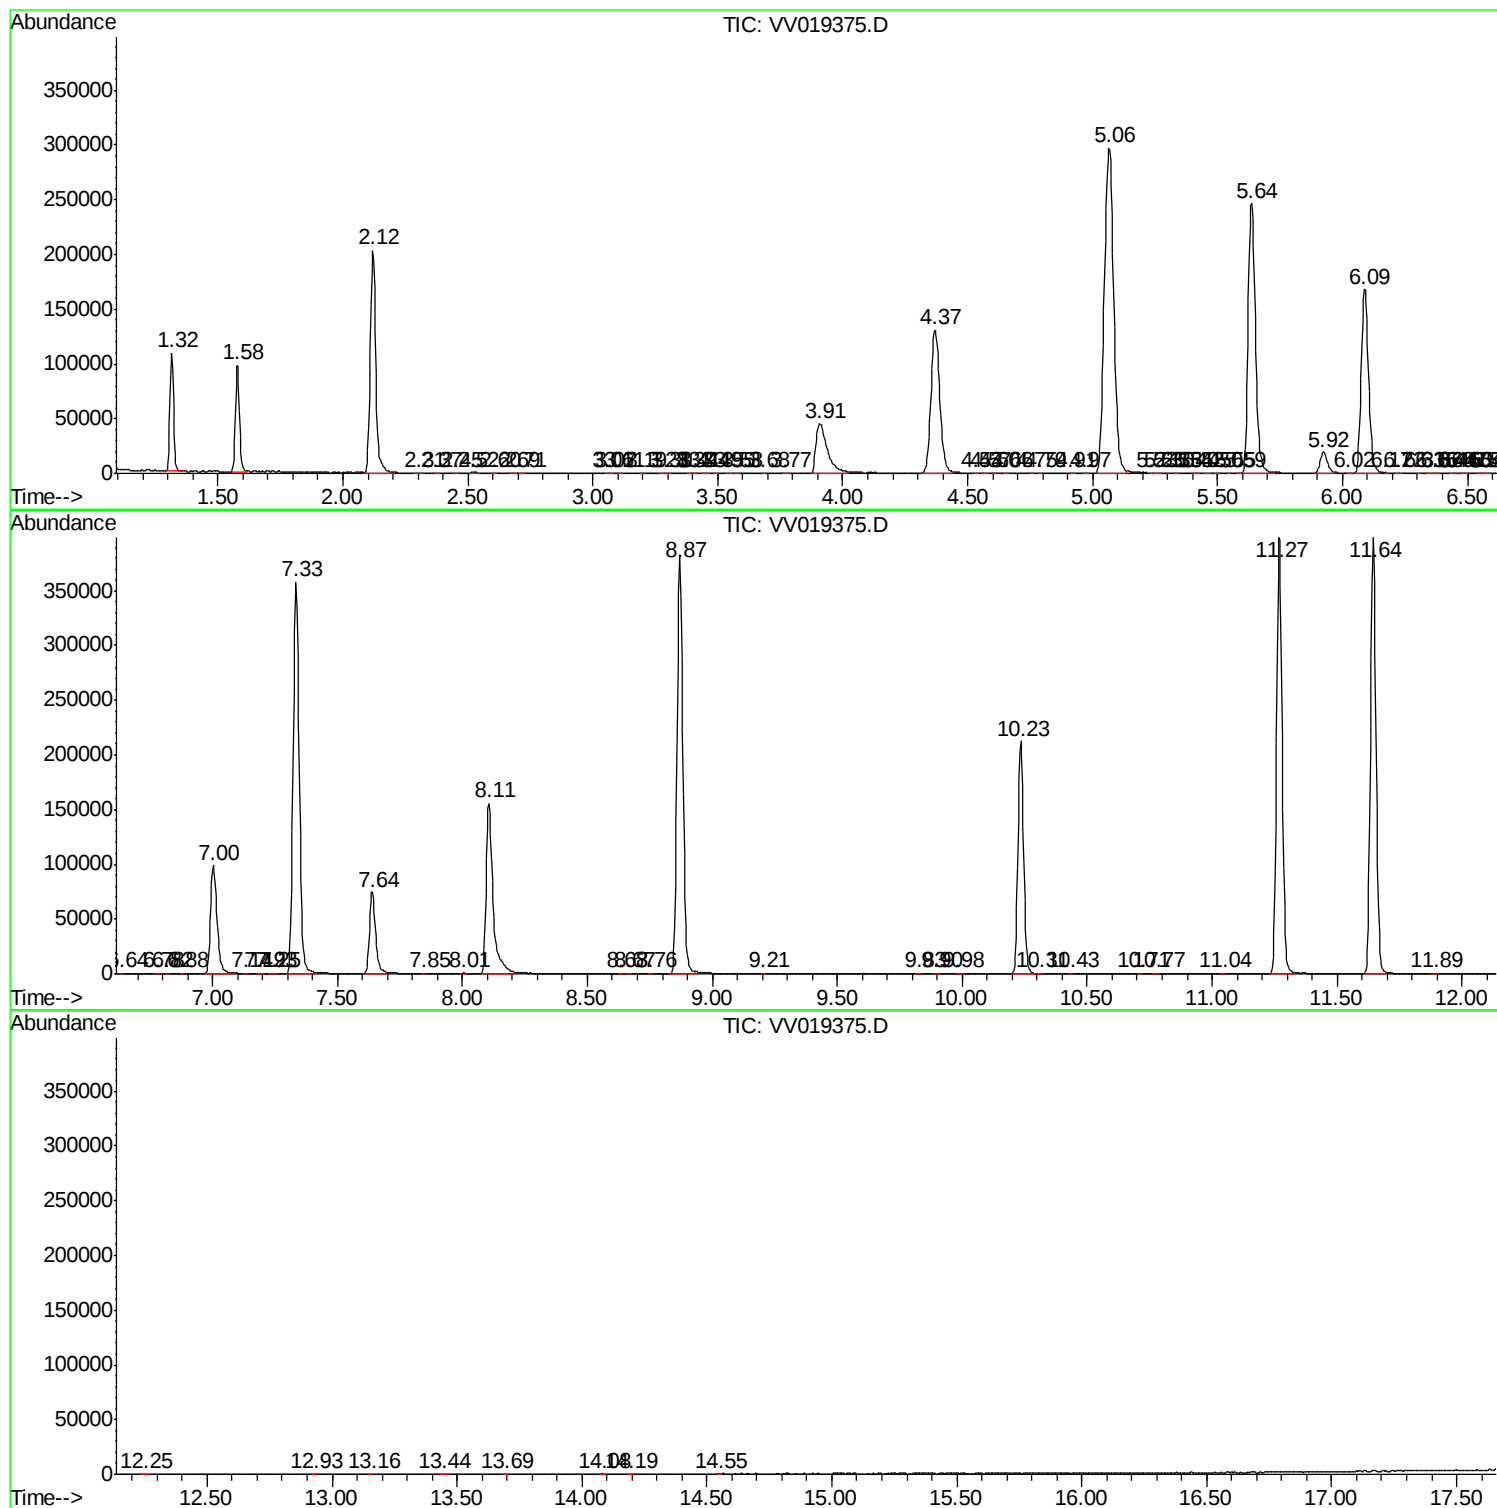

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111320\
Data File : VV019375.D
Acq On : 13 Nov 2020 14:08
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111320\
Data File : VV019375.D
Acq On : 13 Nov 2020 14:08
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK82

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc