

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111323\
 Data File : VW032934.D
 Acq On : 13 Nov 2023 16:14
 Operator : SY/MD
 Sample : 05326-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 14 00:19:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 13 23:16:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	390942	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	396251	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	190934	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	151093	45.696	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	91.400%	
7) Chloroethane-d5	1.532	69	129917	47.423	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.840%	
11) 1,1-Dichloroethene-d2	2.060	65	67789	47.056	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.120%	
21) 2-Butanone-d5	3.786	46	128946	90.980	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	90.980%	
24) Chloroform-d	4.249	84	263226	46.082	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.160%	
26) 1,2-Dichloroethane-d4	4.944	65	164497	47.328	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.660%	
32) Benzene-d6	4.960	84	512526	47.424	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.840%	
36) 1,2-Dichloropropane-d6	5.989	67	152285	48.477	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.960%	
41) Toluene-d8	7.243	98	454284	45.593	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.180%	
43) trans-1,3-Dichloroprop...	7.551	79	71529	42.891	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.780%	
47) 2-Hexanone-d5	8.024	63	109372	95.035	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	95.040%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	208253	45.255	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.500%	
66) 1,2-Dichlorobenzene-d4	11.561	152	186014	50.138	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.280%	
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.912	75	5098	1.141	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032934.D
Acq On : 13 Nov 2023 16:14
Operator : SY/MD
Sample : 05326-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 14 00:19:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 13 23:16:30 2023
Response via : Initial Calibration

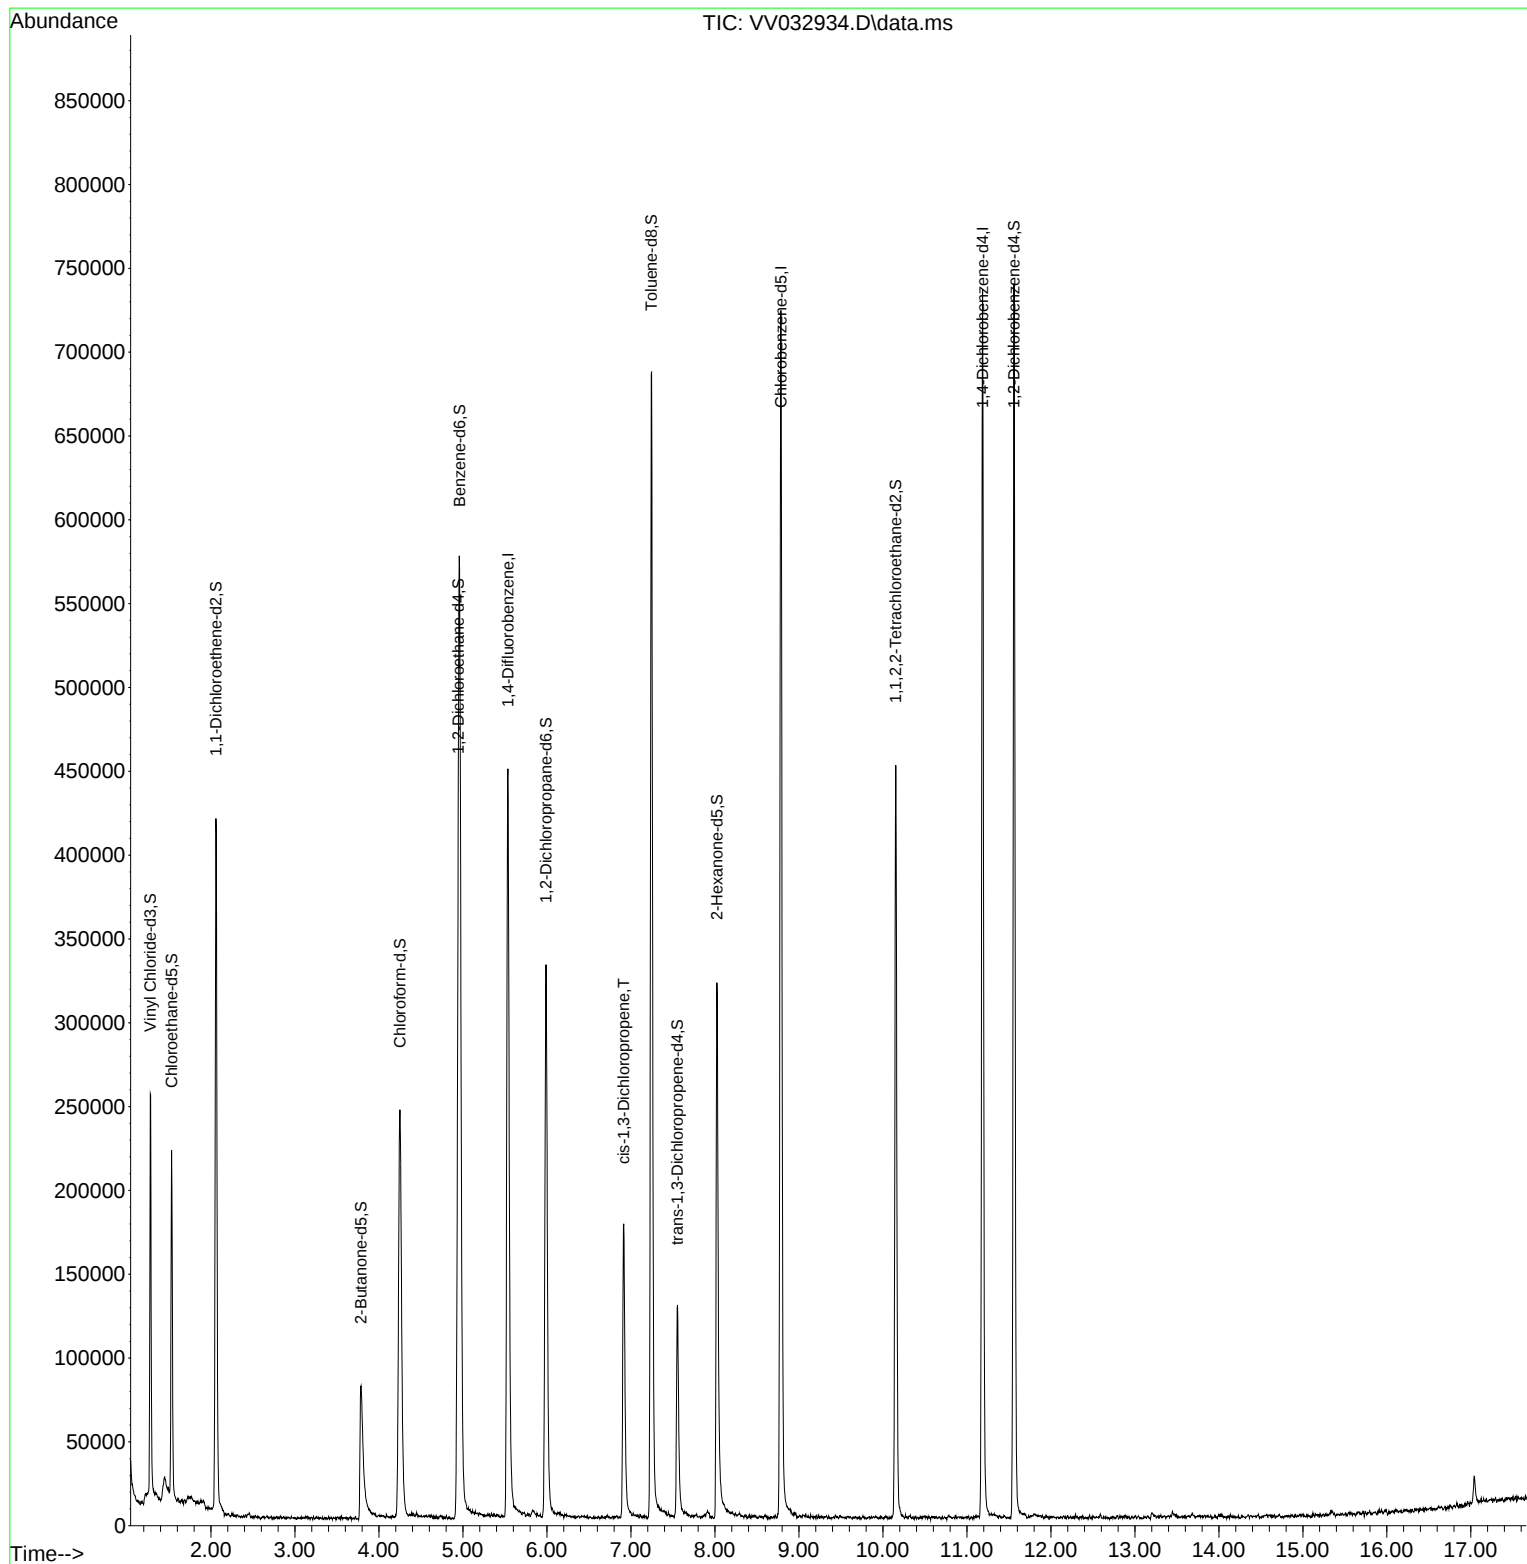

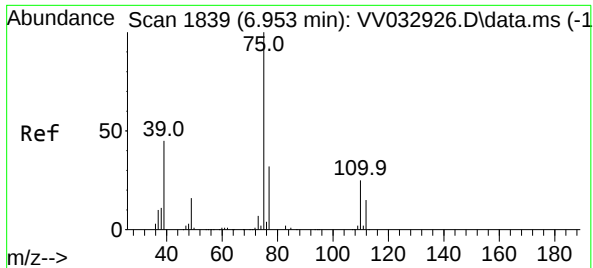

#39
 cis-1,3-Dichloropropene
 Concen: 1.141 ug/L
 RT: 6.912 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV032934.D
 Acq: 13 Nov 2023 16:14

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 5098
 Ion Ratio Lower Upper
 75 100
 77 43.4 21.8 40.6#

