

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111323\
 Data File : VW032949.D
 Acq On : 13 Nov 2023 22:25
 Operator : SY/MD
 Sample : 05296-09 80X
 Misc : 5.96gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3S2

Manual Integrations
 APPROVED

Reviewed By : Mahesh Dadoda 11/17/2023
 Supervised By : Semsettin Yesilyurt 11/17/2023

Quant Time: Nov 14 01:38:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 14 01:11:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	397584	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	391841	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	195925	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	155776	46.326	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	92.660%		
7) Chloroethane-d5	1.532	69	128380	46.079	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.160%		
11) 1,1-Dichloroethene-d2	2.059	65	66445	45.352	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.700%		
21) 2-Butanone-d5	3.783	46	114733	79.600	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.600%		
24) Chloroform-d	4.249	84	267935m	46.122	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.240%		
26) 1,2-Dichloroethane-d4	4.940	65	167317	47.335	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.680%		
32) Benzene-d6	4.960	84	526248	49.242	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.480%		
36) 1,2-Dichloropropane-d6	5.989	67	157126	50.581	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.160%		
41) Toluene-d8	7.243	98	460152	46.701	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.400%		
43) trans-1,3-Dichloroprop...	7.554	79	76600	46.448	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.900%		
47) 2-Hexanone-d5	8.024	63	98057	86.162	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.160%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	212996	46.806	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.620%		
66) 1,2-Dichlorobenzene-d4	11.561	152	193748	50.892	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.780%		
Target Compounds						Qvalue
51) Chlorobenzene	8.818	112	4915	0.611	ug/L #	84
52) Ethylbenzene	8.953	91	47296	3.677	ug/L	98
53) m,p-Xylene	9.072	106	200320	40.508	ug/L	98
54) o-Xylene	9.480	106	114975	24.113	ug/L	97
64) 1,3-Dichlorobenzene	11.127	146	6848	1.132	ug/L	83
65) 1,4-Dichlorobenzene	11.210	146	37061	5.713	ug/L	97
67) 1,2-Dichlorobenzene	11.580	146	14055	2.311	ug/L #	93
70) 1,2,4-trichlorobenzene	13.201	180	93749	22.996	ug/L	99
72) 1,2,3-Trichlorobenzene	13.683	180	42553	10.371	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032949.D
Acq On : 13 Nov 2023 22:25
Operator : SY/MD
Sample : 05296-09 80X
Misc : 5.96gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BH3S2

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023


Quant Time: Nov 14 01:38:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 14 01:11:23 2023
Response via : Initial Calibration

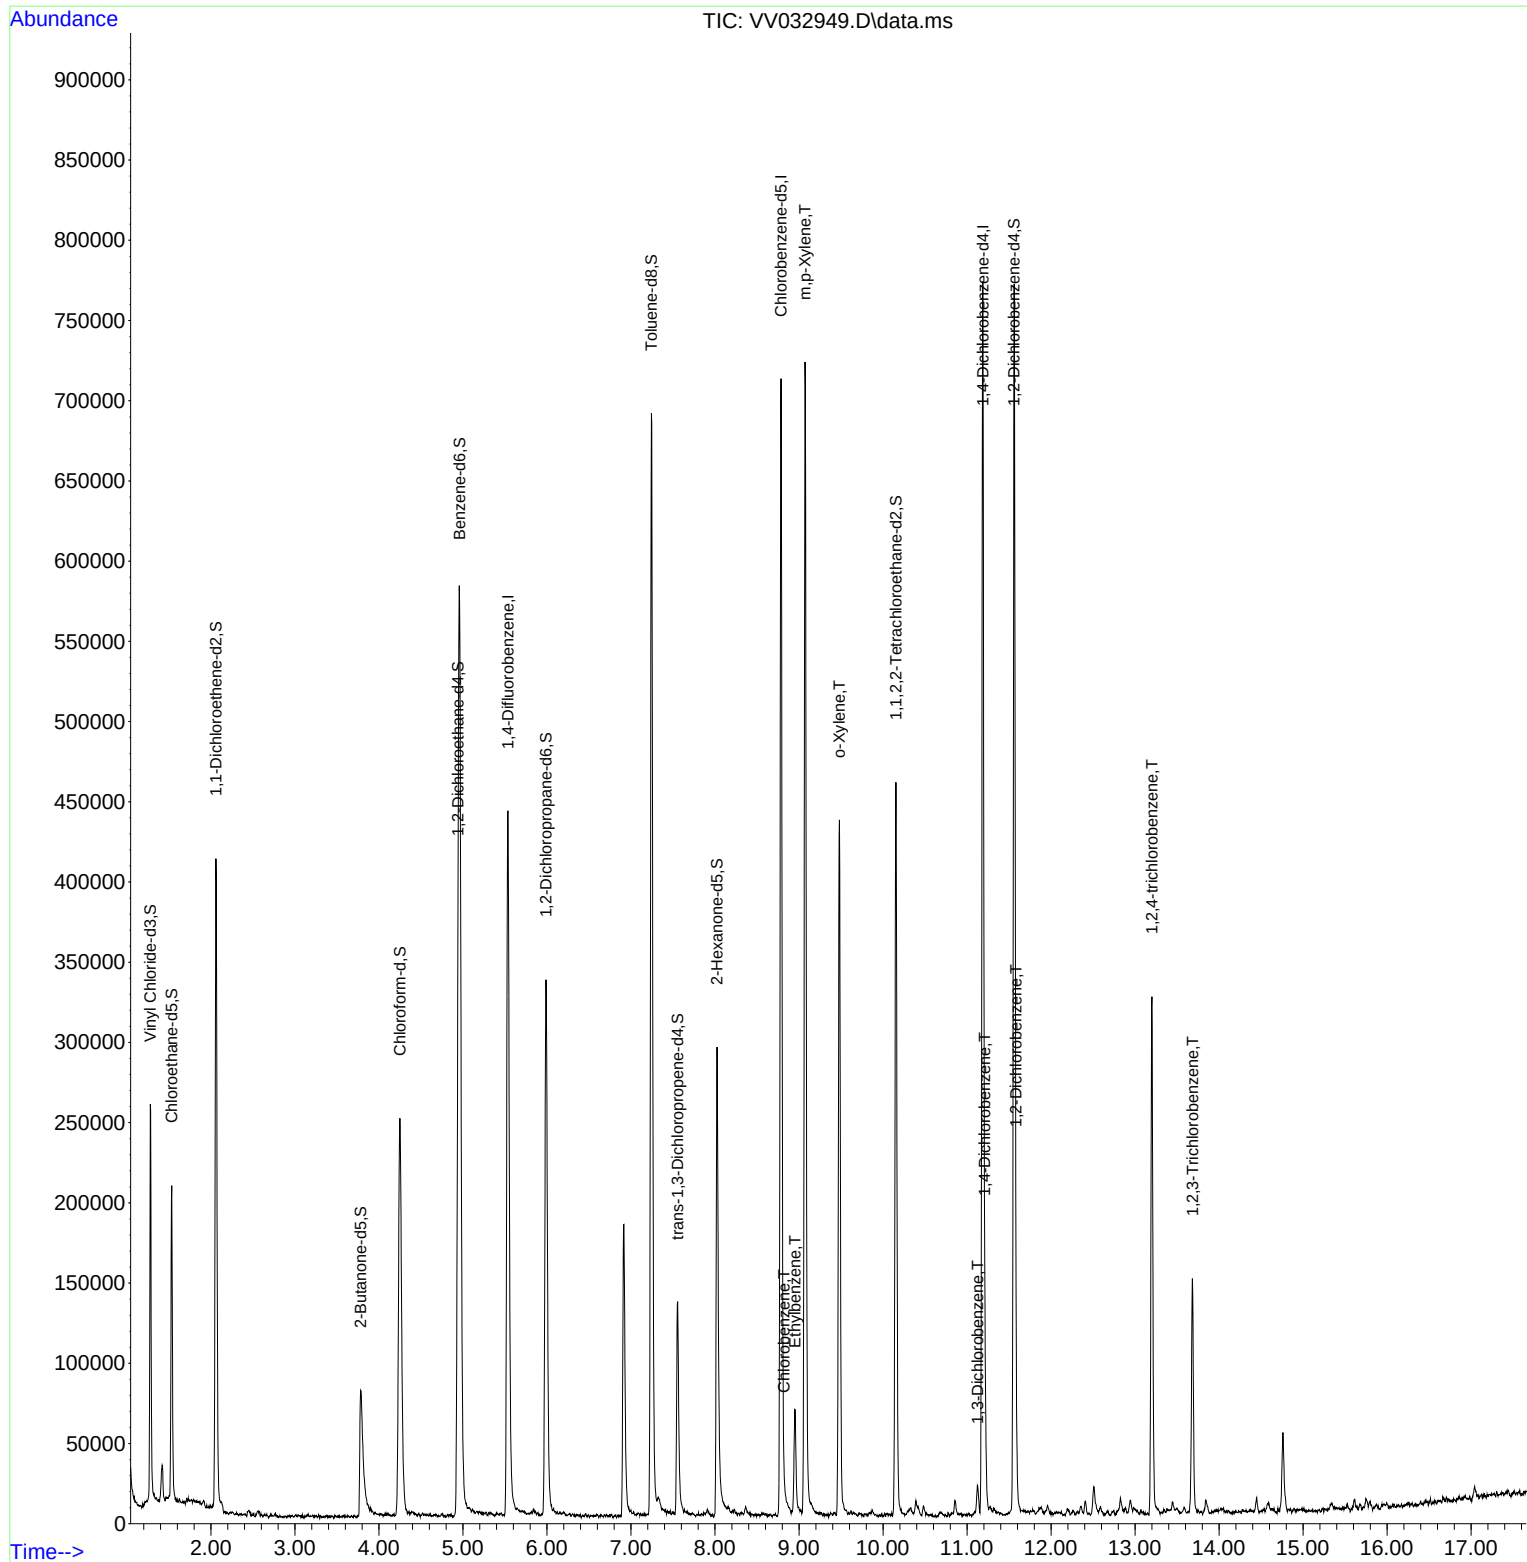

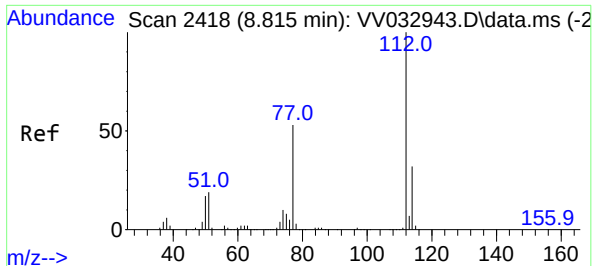

#51
Chlorobenzene
Concen: 0.611 ug/L
RT: 8.818 min Scan# 2418
Delta R.T. 0.003 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25




Instrument :
MSVOA_V
ClientSampleId :
BH3S2

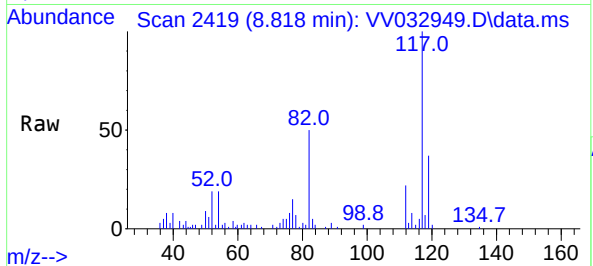

Tgt Ion: 112 Resp: 4915
Ion Ratio Lower Upper
112 100
114 36.6 22.1 41.1
77 69.9 44.2 66.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

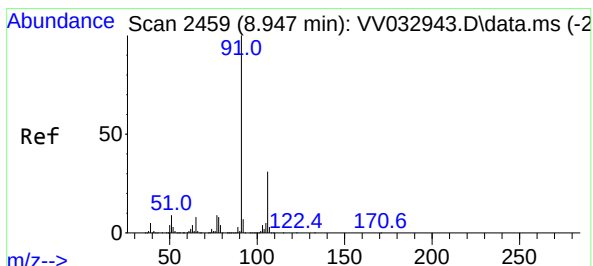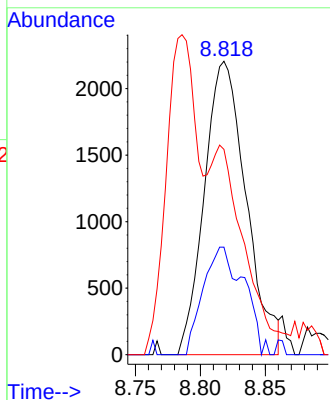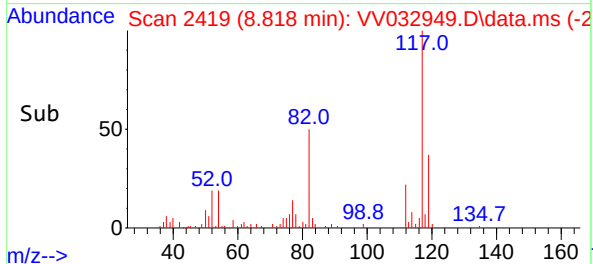

#52
Ethylbenzene
Concen: 3.677 ug/L
RT: 8.953 min Scan# 2461
Delta R.T. 0.006 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25


Tgt Ion: 91 Resp: 47296
Ion Ratio Lower Upper
91 100
106 32.2 21.6 40.0

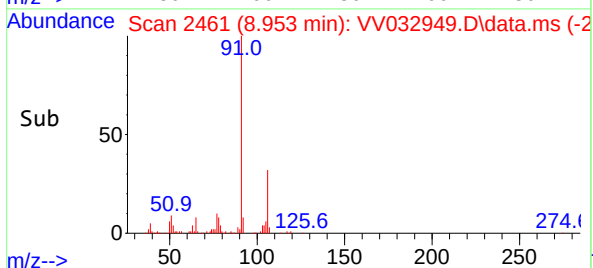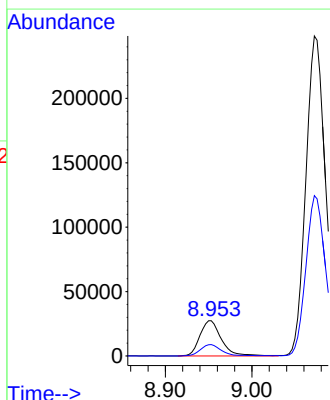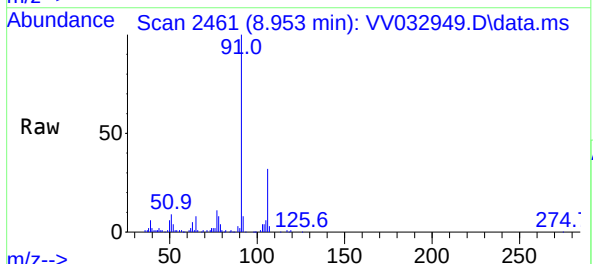

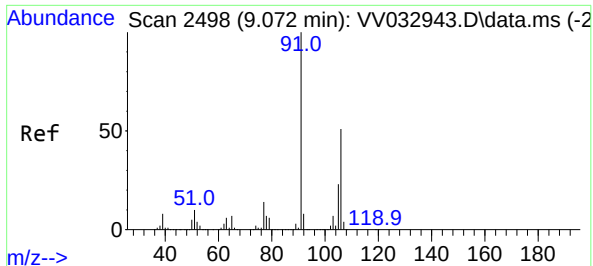

#53
m,p-Xylene
Concen: 40.508 ug/L
RT: 9.072 min Scan# 2498
Delta R.T. -0.000 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25




Instrument :
MSVOA_V
ClientSampleId :
BH3S2

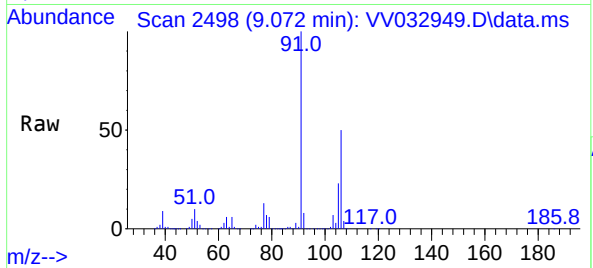


Tgt Ion:106 Resp: 200320
Ion Ratio Lower Upper
106 100
91 199.6 137.5 255.4

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

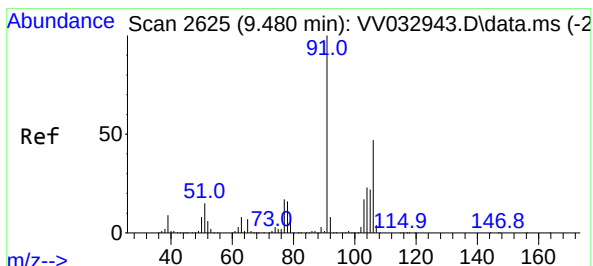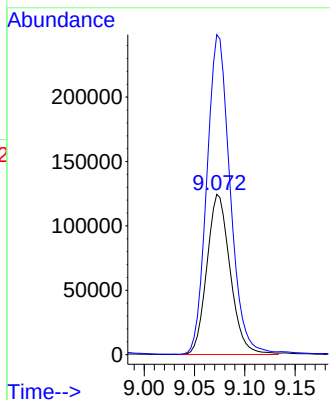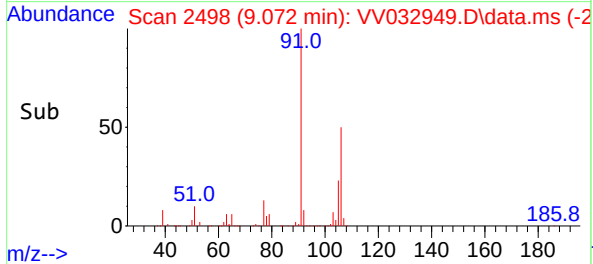


#54
o-Xylene
Concen: 24.113 ug/L
RT: 9.480 min Scan# 2625
Delta R.T. -0.000 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25

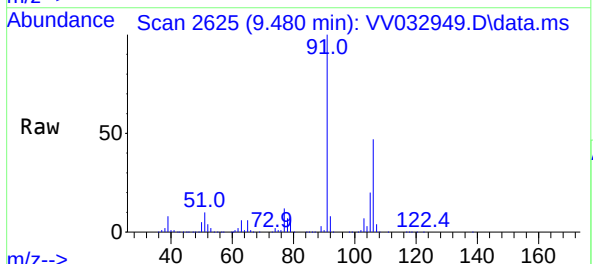


Tgt Ion:106 Resp: 114975
Ion Ratio Lower Upper
106 100
91 211.2 151.6 281.6

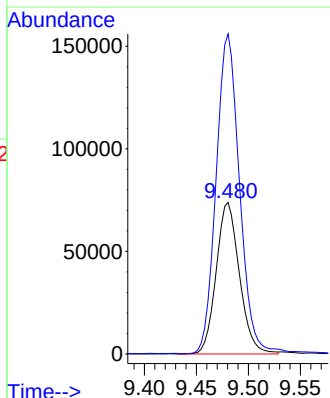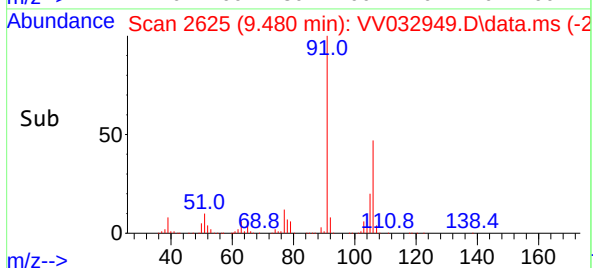

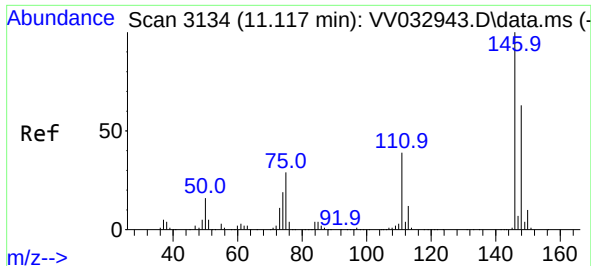

#64
1,3-Dichlorobenzene
Concen: 1.132 ug/L
RT: 11.127 min Scan# 3137
Delta R.T. 0.010 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25




Instrument :
MSVOA_V
ClientSampleId :
BH3S2

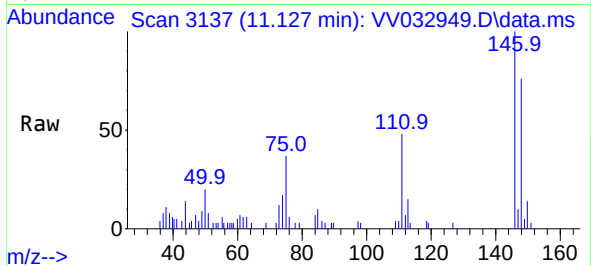


Tgt Ion:146 Resp: 6848
Ion Ratio Lower Upper
146 100
111 48.2 26.9 49.9
148 75.7 43.6 81.0

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

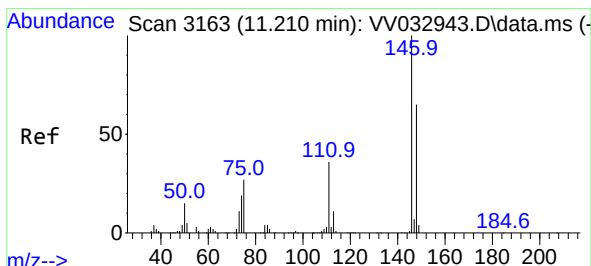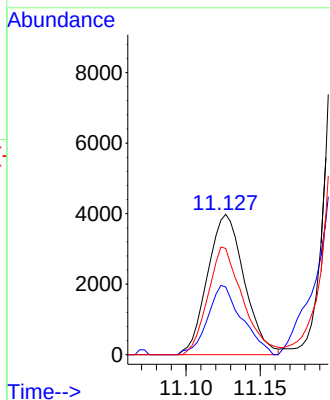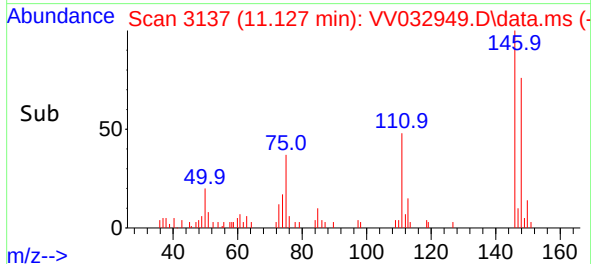


#65
1,4-Dichlorobenzene
Concen: 5.713 ug/L
RT: 11.210 min Scan# 3163
Delta R.T. -0.000 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25

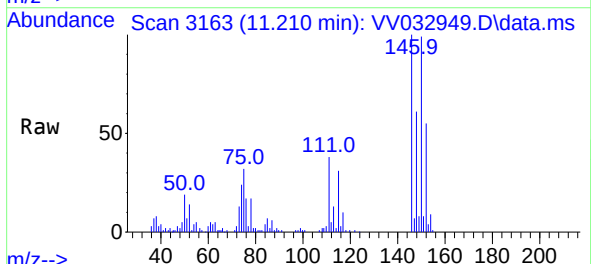

Tgt Ion:146 Resp: 37061
Ion Ratio Lower Upper
146 100
111 38.5 25.5 47.3
148 61.2 44.4 82.5

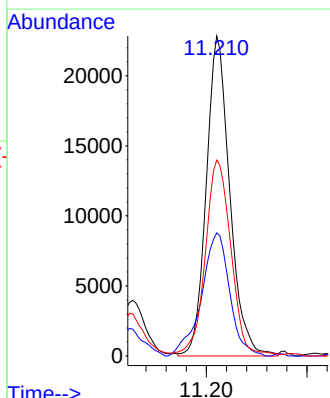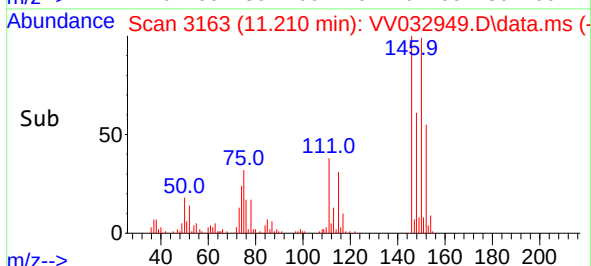

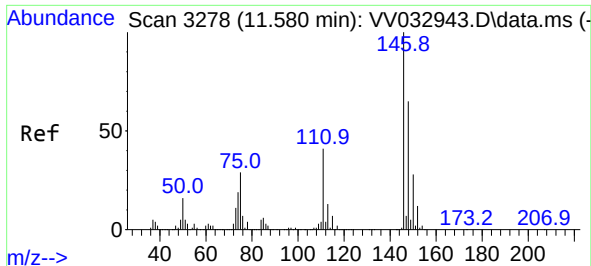

#67

1,2-Dichlorobenzene

Concen: 2.311 ug/L

RT: 11.580 min Scan# 31

Delta R.T. -0.000 min

Lab File: VV032949.D

Acq: 13 Nov 2023 22:25

Instrument :

MSVOA_V

ClientSampleId :





BH3S2

Tgt Ion:	146	Resp:	1405
Ion Ratio	Lower	Upper	
146	100		
111	48.7	31.1	46.7
148	62.4	51.4	77.0

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

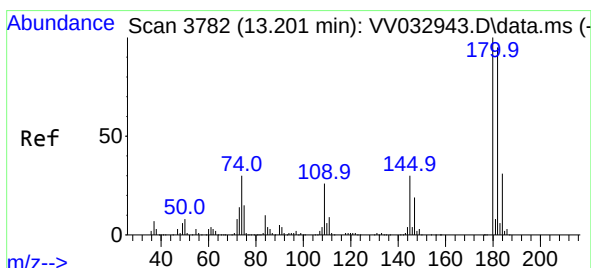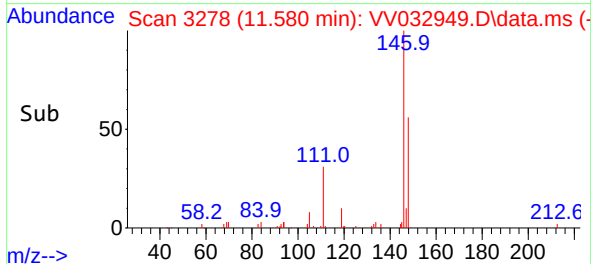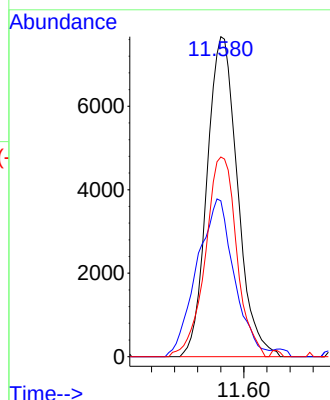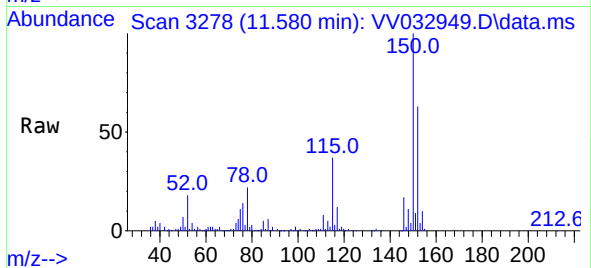

#70

1,2,4-trichlorobenzene

Concen: 22.996 ug/L




RT: 13.201 min Scan# 3782


Delta R.T. -0.000 min

Lab File: VV032949.D

Acq: 13 Nov 2023 22:25


Tgt Ion:	180	Resp:	93749
Ion Ratio	Lower	Upper	
180	100		
182	97.4	77.0	115.4
145	30.9	24.3	36.5

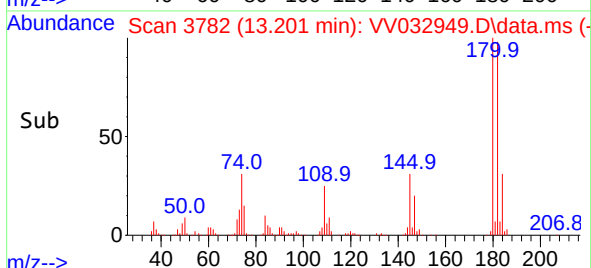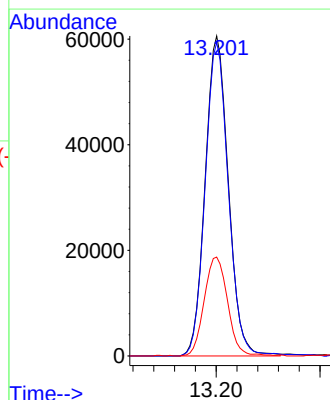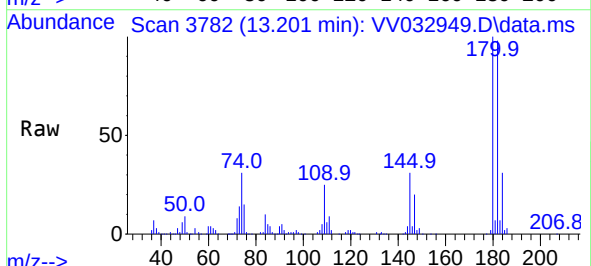

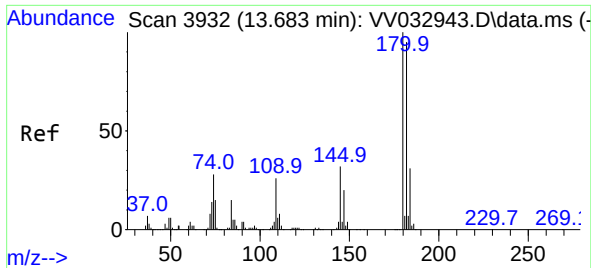

#72
1,2,3-Trichlorobenzene
Concen: 10.371 ug/L
RT: 13.683 min Scan# 3932
Delta R.T. -0.000 min
Lab File: VV032949.D
Acq: 13 Nov 2023 22:25

Instrument :
MSVOA_V
ClientSampleId :
BH3S2

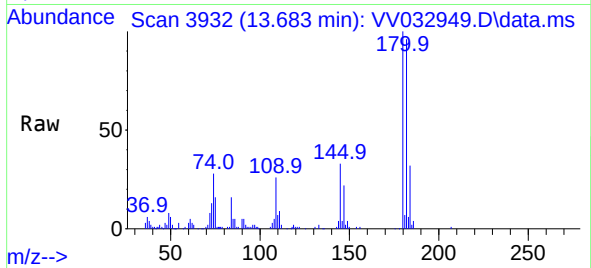

Tgt Ion:180 Resp: 4255
Ion Ratio Lower Upper
180 100
182 95.7 76.9 115.3
145 33.9 26.1 39.1

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 11/17/2023
Supervised By :Semsettin Yesilyurt 11/17/2023

