

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032929.D
 Acq On : 13 Nov 2023 14:18
 Operator : SY/MD
 Sample : VV1113WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	255092	268917	16.85%	2.141%
2	1.532	147	153	168	rVB	211132	245859	15.40%	1.957%
3	2.060	308	317	332	rVB	423968	613921	38.46%	4.887%
4	2.609	484	488	490	rBV5	1704	1336	0.08%	0.011%
5	2.767	534	537	540	rBV5	1383	1123	0.07%	0.009%
6	2.851	561	563	565	rVB4	1166	324	0.02%	0.003%
7	2.925	580	586	587	rBV6	1239	1242	0.08%	0.010%
8	3.005	609	611	612	rBV2	990	379	0.02%	0.003%
9	3.079	632	634	638	rVB5	2085	1547	0.10%	0.012%
10	3.101	638	641	642	rBV3	2058	1220	0.08%	0.010%
11	3.175	659	664	666	rBV6	1986	1642	0.10%	0.013%
12	3.188	666	668	671	rVV3	1475	946	0.06%	0.008%
13	3.207	671	674	680	rVV6	1850	1625	0.10%	0.013%
14	3.246	682	686	691	rBV5	1704	1700	0.11%	0.014%
15	3.416	738	739	741	rBV2	808	224	0.01%	0.002%
16	3.458	749	752	755	rBV5	1468	1153	0.07%	0.009%
17	3.545	775	779	782	rBV6	1621	975	0.06%	0.008%
18	3.587	788	792	797	rBV7	2366	2781	0.17%	0.022%
19	3.635	805	807	810	rVB4	1653	574	0.04%	0.005%
20	3.654	810	813	816	rBV5	1426	984	0.06%	0.008%
21	3.712	829	831	832	rBV	638	303	0.02%	0.002%
22	3.780	843	852	883	rBV	82398	224461	14.06%	1.787%
23	4.098	946	951	953	rBV5	2119	1531	0.10%	0.012%
24	4.246	983	997	1021	rBV	257446	647795	40.58%	5.157%
25	4.953	1201	1217	1241	rBV2	604765	1596251	100.00%	12.708%
26	5.532	1385	1397	1421	rBV	506316	1049226	65.73%	8.353%
27	5.986	1526	1538	1567	rBV	342880	707909	44.35%	5.636%
28	6.584	1722	1724	1727	rBV4	1274	624	0.04%	0.005%
29	6.625	1732	1737	1740	rBV6	2073	2536	0.16%	0.020%
30	6.751	1773	1776	1777	rBV2	2159	1125	0.07%	0.009%
31	6.770	1780	1782	1784	rVV3	1345	638	0.04%	0.005%
32	6.831	1799	1801	1802	rVB2	1153	297	0.02%	0.002%
33	6.912	1815	1826	1844	rBV	193935	365426	22.89%	2.909%
34	7.243	1917	1929	1950	rBV	745369	1306297	81.84%	10.399%
35	7.551	2016	2025	2047	rBV	139859	248898	15.59%	1.981%
36	7.757	2087	2089	2091	rBV3	1619	859	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032929.D
 Acq On : 13 Nov 2023 14:18
 Operator : SY/MD
 Sample : VV1113WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	7.831	2110	2112	2114	rBV3	1224	569	0.04%	0.005%
38	7.982	2158	2159	2162	rBV2	1136	424	0.03%	0.003%
39	8.021	2162	2171	2203	rBV	295117	536035	33.58%	4.267%
40	8.783	2398	2408	2440	rBV	812557	1336388	83.72%	10.639%
41	9.220	2543	2544	2548	rVB4	1628	973	0.06%	0.008%
42	9.246	2548	2552	2553	rBV4	2103	1624	0.10%	0.013%
43	9.345	2580	2583	2586	rBV5	2611	1770	0.11%	0.014%
44	9.558	2646	2649	2650	rBV3	2108	1286	0.08%	0.010%
45	9.587	2656	2658	2661	rVB3	1407	739	0.05%	0.006%
46	9.667	2681	2683	2686	rBV4	1387	1020	0.06%	0.008%
47	9.728	2700	2702	2703	rBV2	1327	341	0.02%	0.003%
48	9.789	2718	2721	2723	rBV4	756	452	0.03%	0.004%
49	9.915	2758	2760	2761	rBV2	1337	494	0.03%	0.004%
50	9.956	2770	2773	2778	rBV6	1610	1313	0.08%	0.010%
51	10.017	2789	2792	2795	rBV4	1639	1148	0.07%	0.009%
52	10.059	2803	2805	2807	rBV3	780	384	0.02%	0.003%
53	10.153	2822	2834	2851	rBV	460824	729540	45.70%	5.808%
54	10.288	2874	2876	2877	rBV2	1475	653	0.04%	0.005%
55	10.484	2933	2937	2938	rBV4	1523	810	0.05%	0.006%
56	10.571	2962	2964	2967	rVB4	1543	778	0.05%	0.006%
57	10.596	2969	2972	2973	rBV3	1181	605	0.04%	0.005%
58	10.609	2973	2976	2979	rVB5	1365	912	0.06%	0.007%
59	10.638	2983	2985	2987	rBV3	1178	759	0.05%	0.006%
60	10.686	2998	3000	3004	rVB5	1231	1010	0.06%	0.008%
61	10.715	3007	3009	3012	rVB3	1456	522	0.03%	0.004%
62	10.738	3012	3016	3021	rBV7	1321	1530	0.10%	0.012%
63	10.763	3022	3024	3028	rBV5	1218	685	0.04%	0.005%
64	10.828	3042	3044	3045	rBV2	928	447	0.03%	0.004%
65	10.860	3051	3054	3057	rBV4	2653	1994	0.12%	0.016%
66	10.905	3066	3068	3070	rBV3	675	221	0.01%	0.002%
67	10.998	3095	3097	3098	rBV2	1108	554	0.03%	0.004%
68	11.082	3121	3123	3126	rVB4	1529	844	0.05%	0.007%
69	11.107	3126	3131	3133	rBV5	2167	1845	0.12%	0.015%
70	11.185	3144	3155	3179	rBV	888420	1358825	85.13%	10.818%
71	11.474	3242	3245	3249	rBV5	1752	1272	0.08%	0.010%
72	11.561	3261	3272	3291	rBV	794262	1250948	78.37%	9.959%
73	11.853	3360	3363	3364	rBV3	995	480	0.03%	0.004%
74	12.146	3452	3454	3455	rBV	1200	527	0.03%	0.004%
75	12.236	3480	3482	3484	rVB3	1922	754	0.05%	0.006%
76	12.583	3585	3590	3595	rBV7	3077	3791	0.24%	0.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032929.D
 Acq On : 13 Nov 2023 14:18
 Operator : SY/MD
 Sample : VV1113WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK219

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	12.657	3611	3613	3615	rBV3	1287	725	0.05%	0.006%
78	12.841	3668	3670	3674	rVB4	1459	828	0.05%	0.007%
79	12.918	3692	3694	3696	rBV3	1354	834	0.05%	0.007%
80	13.008	3718	3722	3724	rBV5	1847	1340	0.08%	0.011%
81	13.313	3813	3817	3819	rVB4	1913	1455	0.09%	0.012%
82	13.326	3819	3821	3822	rBV3	1459	455	0.03%	0.004%
83	13.860	3985	3987	3988	rBV2	1038	370	0.02%	0.003%
84	14.159	4076	4080	4084	rBV6	1884	1847	0.12%	0.015%
85	14.197	4088	4092	4094	rBV5	2200	1197	0.07%	0.010%
86	14.249	4105	4108	4112	rBV6	2336	1591	0.10%	0.013%
87	14.275	4114	4116	4120	rBV5	1783	1051	0.07%	0.008%
88	14.715	4251	4253	4255	rBV2	1467	724	0.05%	0.006%
89	15.004	4341	4343	4345	rBV3	1114	543	0.03%	0.004%
90	15.027	4349	4350	4351	rBV	1296	479	0.03%	0.004%




Sum of corrected areas: 12561353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032929.D
Acq On : 13 Nov 2023 14:18
Operator : SY/MD
Sample : VV1113WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

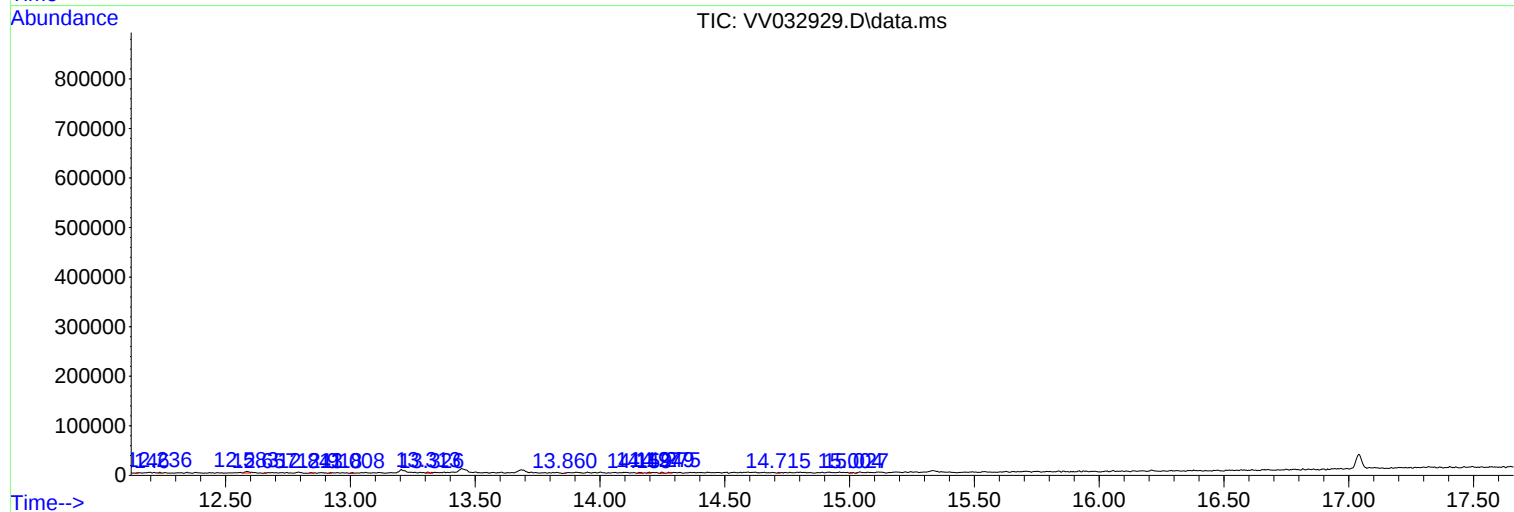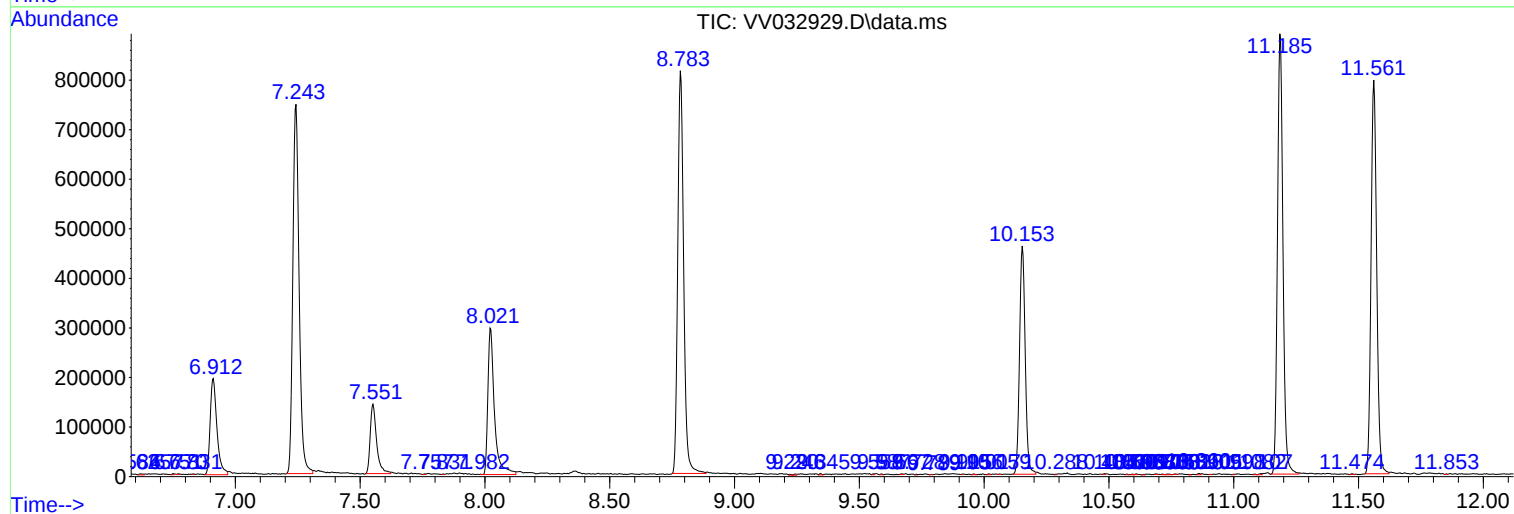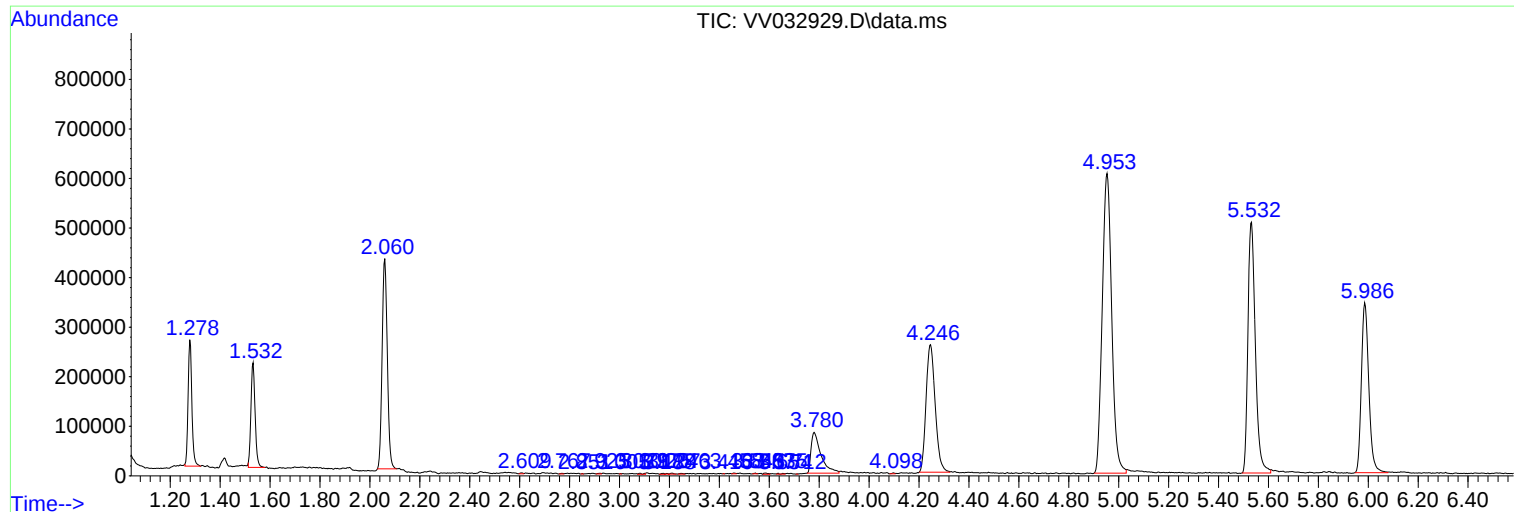

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032929.D
Acq On : 13 Nov 2023 14:18
Operator : SY/MD
Sample : VV1113WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032929.D
Acq On : 13 Nov 2023 14:18
Operator : SY/MD
Sample : VV1113WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK219

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc