

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032930.D
 Acq On : 13 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	246801	263405	17.58%	2.225%
2	1.532	147	153	167	rVB	200427	238549	15.93%	2.015%
3	2.060	308	317	332	rBV	413788	592837	39.58%	5.008%
4	2.230	364	370	373	rBV7	3300	4563	0.30%	0.039%
5	2.616	487	490	493	rBV5	1241	1091	0.07%	0.009%
6	2.867	567	568	573	rVB4	1437	1059	0.07%	0.009%
7	2.963	596	598	602	rVB5	1171	565	0.04%	0.005%
8	3.031	618	619	623	rBV4	847	606	0.04%	0.005%
9	3.191	667	669	671	rBV2	953	560	0.04%	0.005%
10	3.204	671	673	678	rVB5	2258	1521	0.10%	0.013%
11	3.230	678	681	682	rBV3	830	550	0.04%	0.005%
12	3.281	694	697	698	rBV4	1420	657	0.04%	0.006%
13	3.310	704	706	708	rBV3	1190	617	0.04%	0.005%
14	3.371	722	725	729	rVB5	1340	718	0.05%	0.006%
15	3.397	732	733	734	rBV	1990	576	0.04%	0.005%
16	3.407	734	736	739	rVB4	1128	600	0.04%	0.005%
17	3.426	739	742	749	rVB9	1423	1373	0.09%	0.012%
18	3.455	749	751	753	rBV3	1192	689	0.05%	0.006%
19	3.519	767	771	772	rBV4	864	515	0.03%	0.004%
20	3.548	776	780	781	rBV3	1803	1147	0.08%	0.010%
21	3.593	792	794	796	rVB3	1549	658	0.04%	0.006%
22	3.616	796	801	802	rBV4	1626	1247	0.08%	0.011%
23	3.732	834	837	839	rBV4	1006	639	0.04%	0.005%
24	3.783	844	853	880	rBV	78465	211977	14.15%	1.791%
25	4.111	953	955	960	rBV5	1878	1089	0.07%	0.009%
26	4.249	985	998	1022	rVB	240540	602678	40.23%	5.091%
27	4.391	1039	1042	1043	rBV2	2213	1412	0.09%	0.012%
28	4.664	1125	1127	1133	rBV7	1386	1288	0.09%	0.011%
29	4.809	1169	1172	1177	rVB6	1682	1332	0.09%	0.011%
30	4.957	1202	1218	1244	rBV2	569082	1497949	100.00%	12.655%
31	5.420	1360	1362	1367	rBV5	1504	1137	0.08%	0.010%
32	5.535	1386	1398	1420	rBV	475788	976329	65.18%	8.248%
33	5.989	1527	1539	1559	rBV	324045	658601	43.97%	5.564%
34	6.310	1636	1639	1643	rBV5	1476	1402	0.09%	0.012%
35	6.375	1655	1659	1660	rBV3	1667	1208	0.08%	0.010%
36	6.487	1693	1694	1697	rVB3	1386	566	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032930.D
 Acq On : 13 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.571	1717	1720	1727	rBV7	1695	1831	0.12%	0.015%
38	6.603	1727	1730	1732	rBV3	1998	1404	0.09%	0.012%
39	6.725	1766	1768	1769	rBV2	1476	634	0.04%	0.005%
40	6.783	1784	1786	1789	rBV4	1474	737	0.05%	0.006%
41	6.912	1815	1826	1846	rBV	179489	338899	22.62%	2.863%
42	7.092	1880	1882	1885	rVB4	2620	1121	0.07%	0.009%
43	7.243	1918	1929	1951	rBV	691242	1206185	80.52%	10.190%
44	7.487	2003	2005	2012	rVB7	2046	1376	0.09%	0.012%
45	7.551	2017	2025	2047	rVV	128998	229405	15.31%	1.938%
46	7.728	2077	2080	2085	rBV6	2178	1961	0.13%	0.017%
47	7.876	2117	2126	2131	rBV6	3742	7105	0.47%	0.060%
48	8.024	2163	2172	2193	rBV	296305	524638	35.02%	4.432%
49	8.442	2300	2302	2304	rBV3	1675	891	0.06%	0.008%
50	8.645	2363	2365	2367	rBV3	1089	553	0.04%	0.005%
51	8.670	2371	2373	2376	rVB3	1171	623	0.04%	0.005%
52	8.786	2397	2409	2432	rBV	772172	1273968	85.05%	10.763%
53	9.236	2546	2549	2553	rBV5	1818	1815	0.12%	0.015%
54	9.452	2611	2616	2618	rBV6	1758	1851	0.12%	0.016%
55	9.474	2622	2623	2626	rVV3	2071	1023	0.07%	0.009%
56	9.490	2626	2628	2631	rVB4	1432	669	0.04%	0.006%
57	9.509	2631	2634	2635	rBV2	1615	796	0.05%	0.007%
58	9.741	2703	2706	2707	rBV2	1947	1232	0.08%	0.010%
59	9.773	2711	2716	2718	rBV5	1401	1005	0.07%	0.008%
60	9.866	2743	2745	2754	rVB10	3292	4410	0.29%	0.037%
61	9.911	2754	2759	2761	rBV5	1857	1701	0.11%	0.014%
62	9.940	2766	2768	2770	rBV3	1253	537	0.04%	0.005%
63	9.989	2779	2783	2785	rBV4	1512	1162	0.08%	0.010%
64	10.001	2785	2787	2790	rBV4	1359	638	0.04%	0.005%
65	10.063	2802	2806	2808	rBV4	1710	1484	0.10%	0.013%
66	10.153	2821	2834	2851	rBV	450869	715571	47.77%	6.045%
67	10.355	2894	2897	2898	rBV3	1244	835	0.06%	0.007%
68	10.435	2920	2922	2924	rBV4	1061	504	0.03%	0.004%
69	10.693	3000	3002	3005	rBV4	1059	675	0.05%	0.006%
70	10.757	3019	3022	3026	rVB5	1530	1018	0.07%	0.009%
71	10.963	3084	3086	3089	rVB4	1440	764	0.05%	0.006%
72	11.005	3096	3099	3101	rVB4	1357	641	0.04%	0.005%
73	11.085	3119	3124	3127	rBV7	1528	1575	0.11%	0.013%
74	11.111	3127	3132	3133	rBV4	1769	1599	0.11%	0.014%
75	11.185	3145	3155	3175	rBV	802161	1240792	82.83%	10.482%
76	11.487	3245	3249	3251	rBV6	2250	1676	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032930.D
 Acq On : 13 Nov 2023 14:41
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.500	3251	3253	3254	rBV2	1580	556	0.04%	0.005%
78	11.561	3260	3272	3292	rBV	748577	1161756	77.56%	9.815%
79	12.053	3422	3425	3431	rVB6	1453	1492	0.10%	0.013%
80	12.079	3431	3433	3434	rBV2	1059	515	0.03%	0.004%
81	12.194	3467	3469	3471	rVB2	1720	677	0.05%	0.006%
82	12.249	3483	3486	3488	rBV3	1414	990	0.07%	0.008%
83	12.304	3498	3503	3505	rBV6	1692	1638	0.11%	0.014%
84	12.587	3585	3591	3594	rBV8	3658	3868	0.26%	0.033%
85	12.680	3617	3620	3621	rBV2	1128	560	0.04%	0.005%
86	12.725	3631	3634	3638	rBV5	1467	1418	0.09%	0.012%
87	12.744	3638	3640	3641	rBV2	1566	672	0.04%	0.006%
88	12.956	3702	3706	3709	rVB5	1512	1324	0.09%	0.011%
89	12.976	3709	3712	3716	rVB6	1513	948	0.06%	0.008%
90	12.998	3716	3719	3720	rBV3	1646	994	0.07%	0.008%
91	13.024	3725	3727	3730	rBV4	1764	1081	0.07%	0.009%
92	13.043	3730	3733	3736	rVB4	1437	950	0.06%	0.008%
93	13.066	3736	3740	3743	rBV6	2573	1781	0.12%	0.015%
94	13.082	3743	3745	3748	rVB4	1347	630	0.04%	0.005%
95	13.101	3748	3751	3752	rBV3	1397	728	0.05%	0.006%
96	13.554	3889	3892	3895	rBV4	1695	1093	0.07%	0.009%
97	13.599	3903	3906	3910	rBV5	2017	1683	0.11%	0.014%
98	14.281	4115	4118	4119	rBV3	1727	815	0.05%	0.007%
99	14.496	4183	4185	4192	rBV7	2004	1821	0.12%	0.015%
100	14.902	4308	4311	4316	rBV6	2305	2015	0.13%	0.017%




Sum of corrected areas: 11837019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032930.D
Acq On : 13 Nov 2023 14:41
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

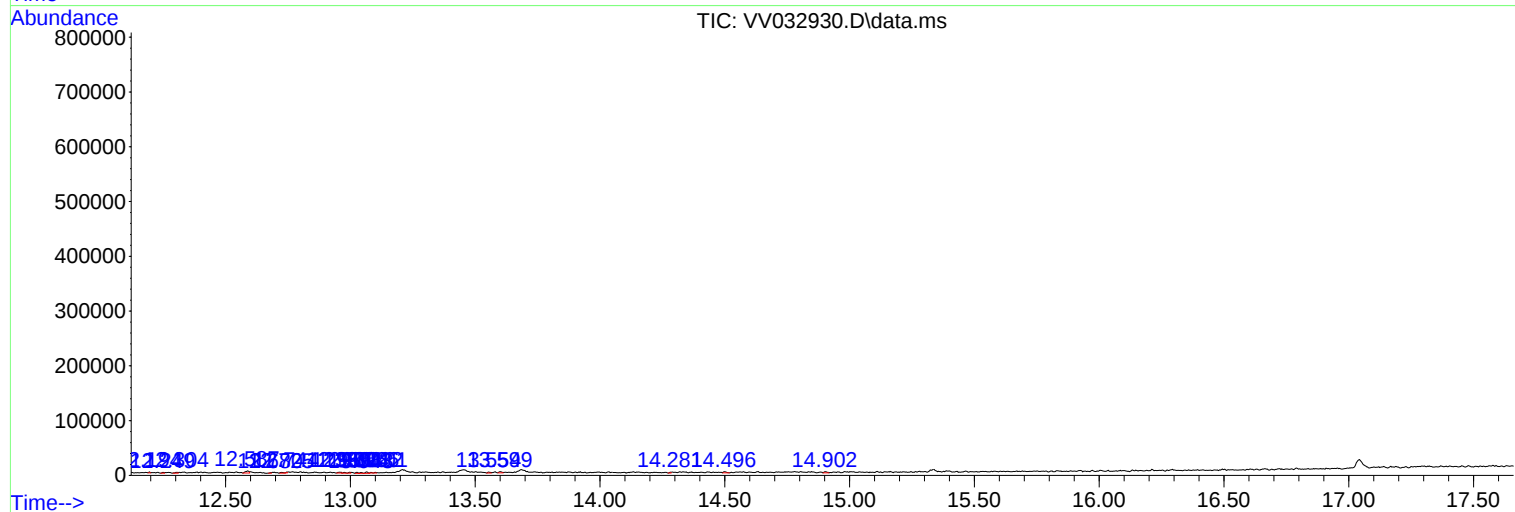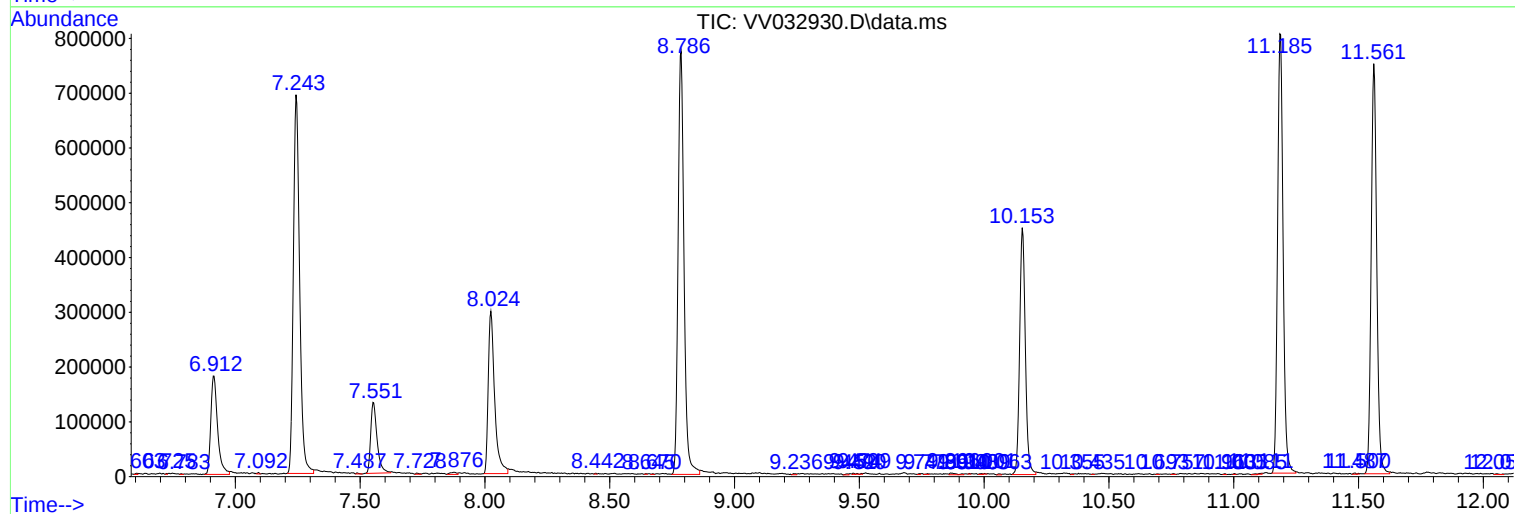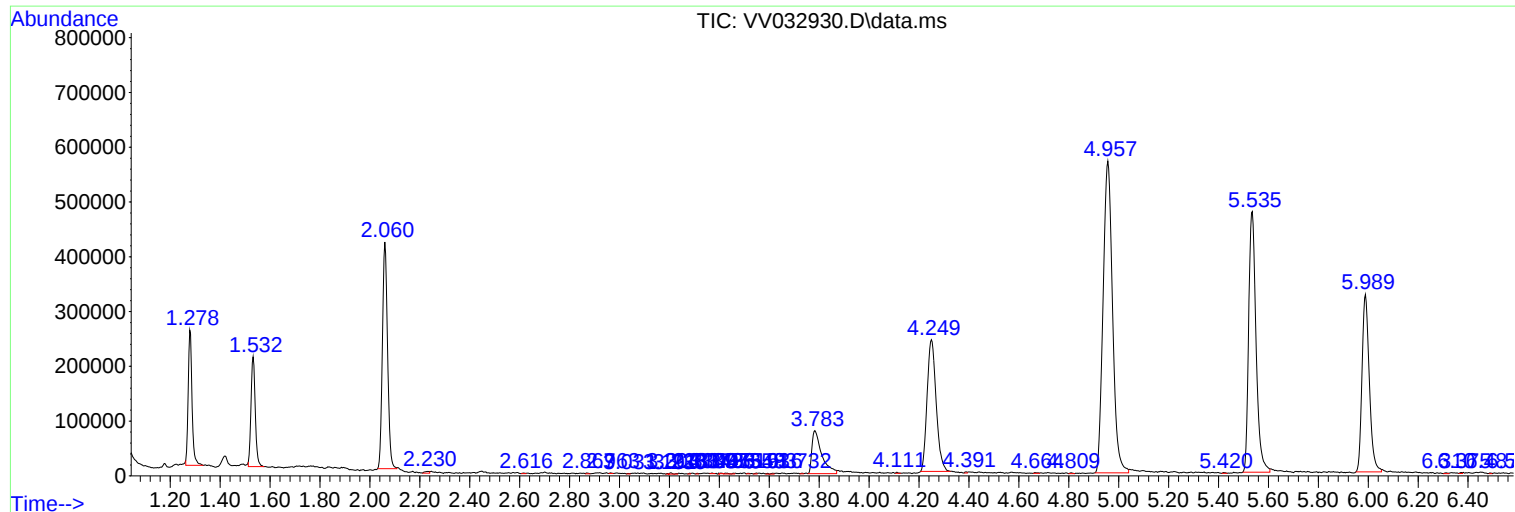

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032930.D
Acq On : 13 Nov 2023 14:41
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032930.D
Acq On : 13 Nov 2023 14:41
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------