

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032931.D
 Acq On : 13 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	91	rVB	251740	267236	17.21%	2.219%
2	1.532	147	153	167	rVB	207779	250177	16.11%	2.078%
3	2.060	308	317	331	rBV	420348	615805	39.66%	5.114%
4	2.490	448	451	453	rBV3	1063	844	0.05%	0.007%
5	2.609	486	488	490	rBV2	1148	711	0.05%	0.006%
6	2.764	534	536	538	rBV3	1066	749	0.05%	0.006%
7	2.831	555	557	559	rBV3	705	354	0.02%	0.003%
8	2.863	565	567	569	rVB4	1078	425	0.03%	0.004%
9	2.937	587	590	591	rBV3	1600	807	0.05%	0.007%
10	2.947	591	593	595	rBV3	997	512	0.03%	0.004%
11	2.976	600	602	604	rBV3	1111	488	0.03%	0.004%
12	3.021	614	616	617	rBV2	815	228	0.01%	0.002%
13	3.076	630	633	636	rBV4	1375	974	0.06%	0.008%
14	3.092	636	638	641	rVB3	1391	578	0.04%	0.005%
15	3.108	641	643	647	rVB5	1547	762	0.05%	0.006%
16	3.130	647	650	652	rVB4	1157	687	0.04%	0.006%
17	3.153	655	657	659	rVB3	816	317	0.02%	0.003%
18	3.175	659	664	670	rBV10	2183	2557	0.16%	0.021%
19	3.214	670	676	678	rBV7	1772	1489	0.10%	0.012%
20	3.227	678	680	682	rBV3	731	322	0.02%	0.003%
21	3.240	682	684	688	rVB4	1627	938	0.06%	0.008%
22	3.259	688	690	692	rBV3	1101	469	0.03%	0.004%
23	3.333	710	713	714	rBV3	1031	653	0.04%	0.005%
24	3.407	733	736	741	rBV6	2085	2196	0.14%	0.018%
25	3.478	754	758	760	rBV5	1783	1202	0.08%	0.010%
26	3.500	763	765	767	rBV3	1436	871	0.06%	0.007%
27	3.593	792	794	799	rBV6	1168	656	0.04%	0.005%
28	3.629	802	805	809	rVB6	1213	1067	0.07%	0.009%
29	3.648	809	811	812	rBV2	862	306	0.02%	0.003%
30	3.658	812	814	816	rBV3	1077	522	0.03%	0.004%
31	3.722	831	834	836	rBV4	1735	1026	0.07%	0.009%
32	3.783	844	853	876	rBV2	81581	220420	14.20%	1.831%
33	4.249	982	998	1022	rBV	248983	639337	41.18%	5.310%
34	4.773	1158	1161	1163	rBV3	1238	899	0.06%	0.007%
35	4.802	1168	1170	1171	rBV2	646	266	0.02%	0.002%
36	4.815	1171	1174	1176	rVV4	1282	649	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111323\
 Data File : VW032931.D
 Acq On : 13 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	4.825	1176	1177	1180	rVB3	1156	396	0.03%	0.003%
38	4.957	1201	1218	1247	rBV2	584018	1552580	100.00%	12.894%
39	5.535	1386	1398	1421	rBV	468906	953881	61.44%	7.922%
40	5.989	1528	1539	1568	rVB	331809	678199	43.68%	5.632%
41	6.211	1607	1608	1612	rBV2	1464	874	0.06%	0.007%
42	6.442	1677	1680	1683	rBV5	1762	1271	0.08%	0.011%
43	6.606	1725	1731	1732	rBV5	1718	1406	0.09%	0.012%
44	6.622	1734	1736	1738	rBV3	1550	959	0.06%	0.008%
45	6.706	1758	1762	1763	rBV3	1996	1285	0.08%	0.011%
46	6.741	1771	1773	1775	rBV3	1084	587	0.04%	0.005%
47	6.802	1790	1792	1795	rVB2	1447	865	0.06%	0.007%
48	6.825	1795	1799	1800	rBV4	1255	629	0.04%	0.005%
49	6.912	1812	1826	1850	rBV	184883	355804	22.92%	2.955%
50	7.243	1918	1929	1957	rBV	710449	1256774	80.95%	10.437%
51	7.551	2017	2025	2049	rBV2	133295	245294	15.80%	2.037%
52	8.024	2162	2172	2197	rBV	321094	566616	36.50%	4.706%
53	8.490	2315	2317	2318	rBV2	978	405	0.03%	0.003%
54	8.680	2374	2376	2378	rBV3	852	333	0.02%	0.003%
55	8.786	2397	2409	2431	rBV	753107	1227294	79.05%	10.193%
56	9.072	2495	2498	2501	rBV4	2418	1763	0.11%	0.015%
57	9.252	2552	2554	2556	rVB3	1075	348	0.02%	0.003%
58	9.265	2556	2558	2559	rBV2	1087	366	0.02%	0.003%
59	9.355	2582	2586	2587	rBV4	1218	908	0.06%	0.008%
60	9.448	2613	2615	2620	rBV6	1935	1919	0.12%	0.016%
61	9.484	2624	2626	2627	rBV2	1606	705	0.05%	0.006%
62	9.538	2641	2643	2645	rBV3	1246	730	0.05%	0.006%
63	9.587	2653	2658	2661	rBV5	1065	1212	0.08%	0.010%
64	9.606	2662	2664	2665	rBV2	1902	644	0.04%	0.005%
65	9.680	2684	2687	2688	rBV3	978	461	0.03%	0.004%
66	9.699	2691	2693	2696	rVV3	1440	824	0.05%	0.007%
67	9.722	2698	2700	2703	rVV4	1521	727	0.05%	0.006%
68	9.741	2703	2706	2711	rVB6	1730	1151	0.07%	0.010%
69	9.828	2731	2733	2734	rBV2	1251	432	0.03%	0.004%
70	9.866	2739	2745	2747	rBV6	2352	1834	0.12%	0.015%
71	9.924	2761	2763	2765	rBV3	1156	471	0.03%	0.004%
72	9.937	2765	2767	2772	rVB6	1122	736	0.05%	0.006%
73	10.153	2821	2834	2856	rBV	470624	745947	48.05%	6.195%
74	10.448	2922	2926	2932	rVB9	2503	2608	0.17%	0.022%
75	10.477	2932	2935	2936	rBV3	1718	1001	0.06%	0.008%
76	10.593	2968	2971	2976	rBV8	2424	2049	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032931.D
 Acq On : 13 Nov 2023 15:04
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	10.619	2977	2979	2982	rBV4	927	587	0.04%	0.005%
78	10.689	2995	3001	3004	rBV7	1490	1762	0.11%	0.015%
79	10.940	3076	3079	3080	rBV3	1984	1033	0.07%	0.009%
80	11.059	3113	3116	3120	rBV4	1114	899	0.06%	0.007%
81	11.185	3145	3155	3179	rBV	773296	1215077	78.26%	10.091%
82	11.561	3261	3272	3294	rVB	752966	1176771	75.79%	9.773%
83	12.149	3453	3455	3457	rBV3	1727	1037	0.07%	0.009%
84	12.178	3462	3464	3466	rVV3	1258	575	0.04%	0.005%
85	12.641	3606	3608	3610	rBV2	1212	728	0.05%	0.006%
86	12.670	3615	3617	3619	rBV3	1878	928	0.06%	0.008%
87	12.914	3690	3693	3694	rBV3	1350	672	0.04%	0.006%
88	13.101	3748	3751	3753	rBV4	812	493	0.03%	0.004%
89	13.117	3753	3756	3758	rVV4	1467	935	0.06%	0.008%
90	13.152	3762	3767	3768	rBV5	1467	886	0.06%	0.007%
91	13.297	3810	3812	3813	rBV2	1429	467	0.03%	0.004%
92	13.339	3823	3825	3826	rBV2	1406	485	0.03%	0.004%
93	13.660	3923	3925	3927	rBV3	2349	1331	0.09%	0.011%
94	13.943	4011	4013	4017	rBV5	1593	978	0.06%	0.008%
95	13.976	4021	4023	4025	rBV3	1265	562	0.04%	0.005%
96	14.046	4043	4045	4047	rBV3	1471	653	0.04%	0.005%
97	14.252	4108	4109	4110	rBV2	1289	405	0.03%	0.003%
98	14.384	4148	4150	4153	rBV4	1428	891	0.06%	0.007%
99	14.712	4250	4252	4253	rBV2	1452	489	0.03%	0.004%
100	15.066	4359	4362	4367	rBV7	2823	2552	0.16%	0.021%




Sum of corrected areas: 12040983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032931.D
Acq On : 13 Nov 2023 15:04
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

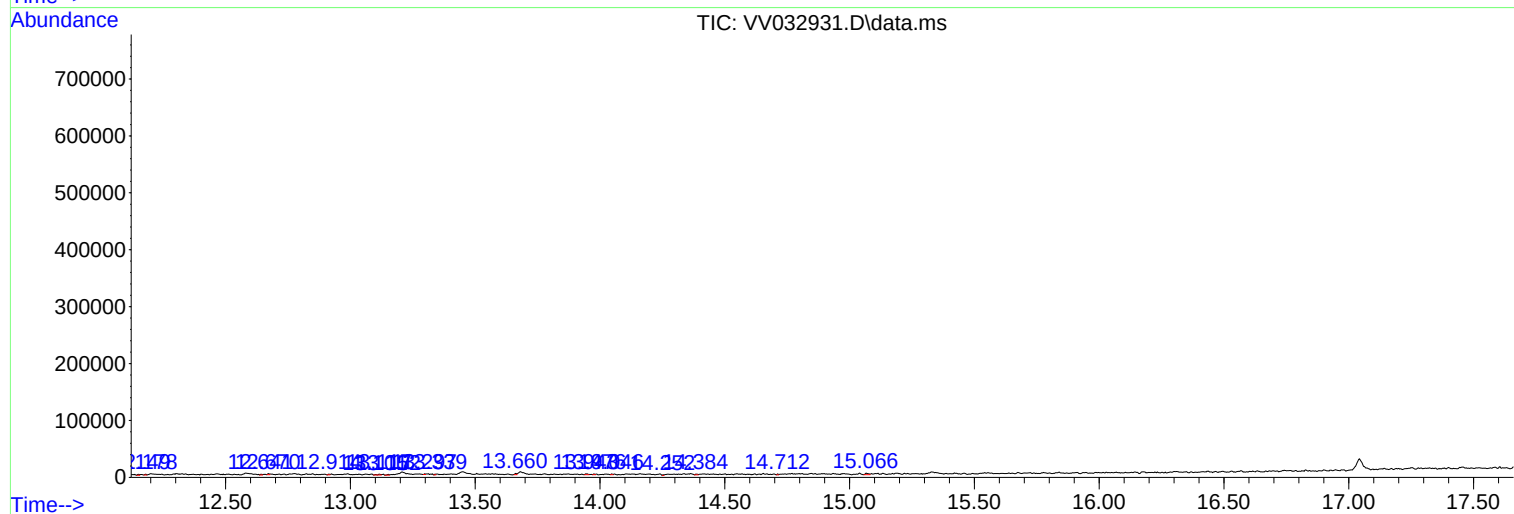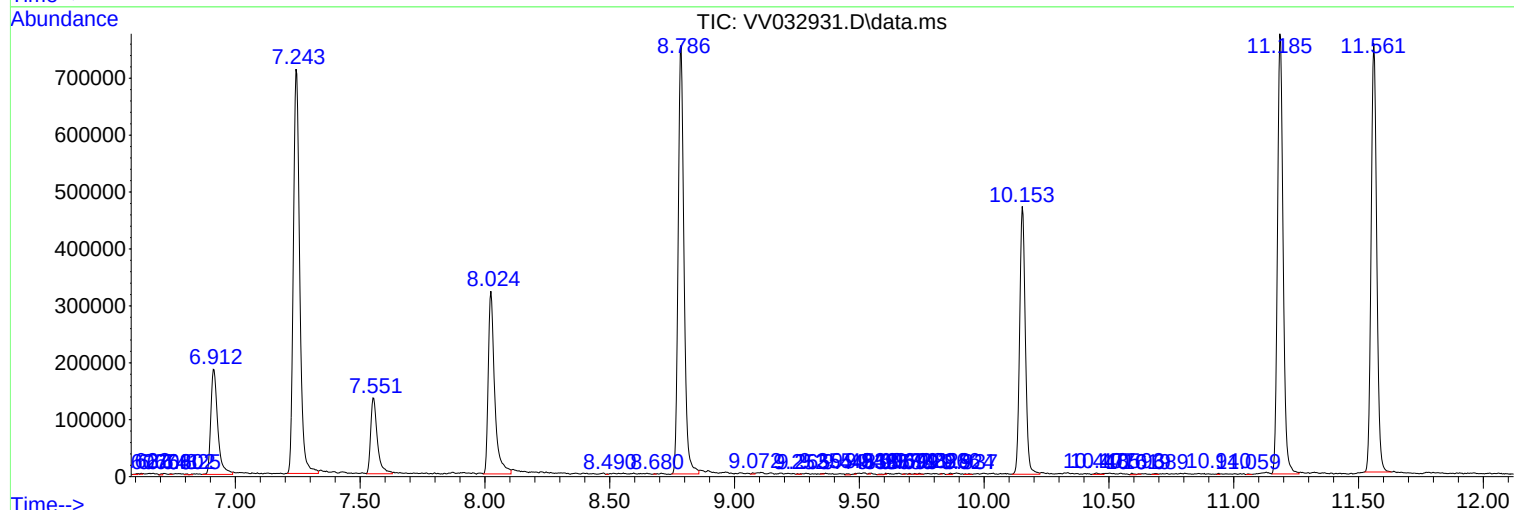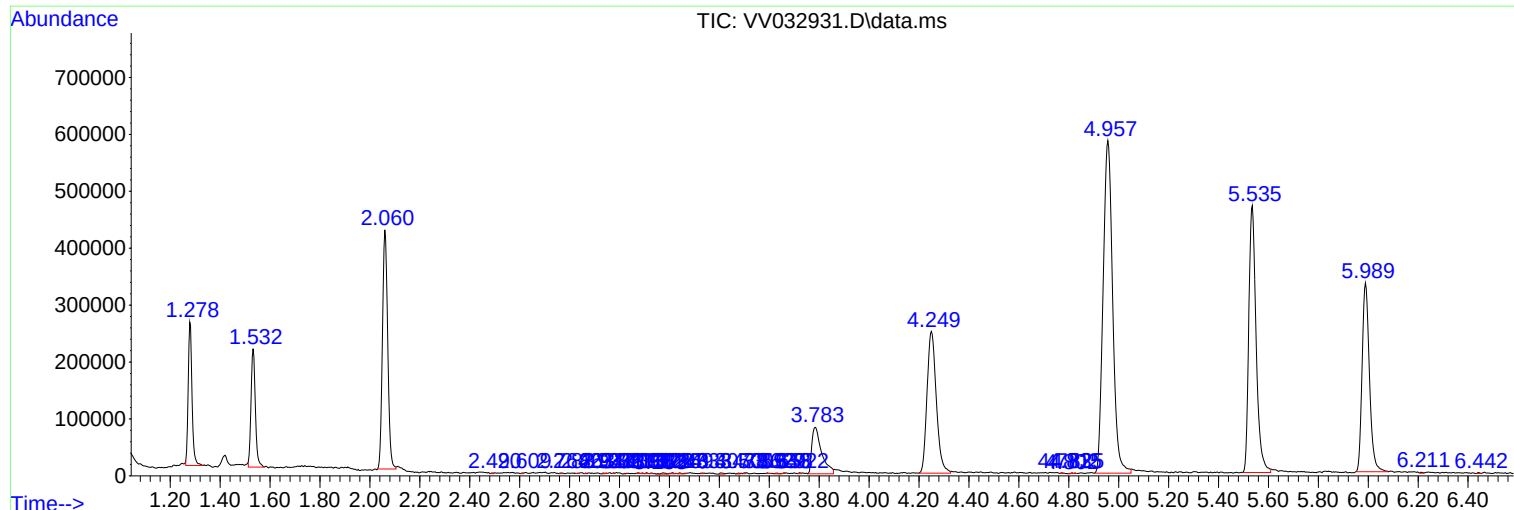

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032931.D
Acq On : 13 Nov 2023 15:04
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032931.D
Acq On : 13 Nov 2023 15:04
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc