

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032933.D
 Acq On : 13 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05326-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	90	rVB	240782	255187	16.84%	1.957%
2	1.532	147	153	169	rVB	198918	240400	15.86%	1.843%
3	2.059	308	317	331	rBV	404166	584413	38.56%	4.481%
4	2.400	421	423	428	rBV4	1590	1592	0.11%	0.012%
5	2.641	492	498	500	rBV6	1923	1940	0.13%	0.015%
6	2.751	531	532	536	rVB3	893	431	0.03%	0.003%
7	2.780	536	541	544	rBV6	1384	1311	0.09%	0.010%
8	2.796	544	546	551	rBV6	1639	1326	0.09%	0.010%
9	2.854	560	564	565	rBV3	1347	896	0.06%	0.007%
10	3.024	613	617	622	rVB6	1952	1862	0.12%	0.014%
11	3.050	622	625	626	rVV2	715	355	0.02%	0.003%
12	3.066	628	630	633	rVV3	2052	990	0.07%	0.008%
13	3.082	633	635	638	rVV4	2135	973	0.06%	0.007%
14	3.101	639	641	644	rVB4	1801	850	0.06%	0.007%
15	3.172	659	663	665	rBV4	1974	1322	0.09%	0.010%
16	3.220	676	678	680	rBV3	2338	1108	0.07%	0.008%
17	3.252	687	688	691	rBV2	864	419	0.03%	0.003%
18	3.268	691	693	696	rBV4	1476	689	0.05%	0.005%
19	3.387	728	730	732	rBV3	958	423	0.03%	0.003%
20	3.420	737	740	741	rBV2	1396	824	0.05%	0.006%
21	3.468	754	755	758	rVB3	1208	565	0.04%	0.004%
22	3.484	758	760	764	rBV5	919	663	0.04%	0.005%
23	3.513	767	769	771	rBV3	926	581	0.04%	0.004%
24	3.593	792	794	800	rVB7	1885	1343	0.09%	0.010%
25	3.619	800	802	803	rBV2	1295	506	0.03%	0.004%
26	3.703	824	828	829	rBV4	1646	1017	0.07%	0.008%
27	3.783	843	853	879	rBV2	85712	238708	15.75%	1.830%
28	4.249	984	998	1022	rBV	243966	614764	40.56%	4.714%
29	4.957	1200	1218	1246	rBV2	570701	1515539	100.00%	11.621%
30	5.477	1378	1380	1384	rVB5	2389	1303	0.09%	0.010%
31	5.535	1386	1398	1421	rBV	450380	933187	61.57%	7.156%
32	5.989	1528	1539	1563	rVB2	322070	659683	43.53%	5.059%
33	6.555	1713	1715	1717	rBV3	918	437	0.03%	0.003%
34	6.696	1757	1759	1763	rVB4	1837	814	0.05%	0.006%
35	6.744	1772	1774	1775	rBV2	963	357	0.02%	0.003%
36	6.792	1786	1789	1790	rBV4	1883	914	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032933.D
 Acq On : 13 Nov 2023 15:51
 Operator : SY/MD
 Sample : 05326-02DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.818	1794	1797	1801	rBV5	1490	1196	0.08%	0.009%
38	6.915	1817	1827	1844	rBV	180578	331953	21.90%	2.545%
39	7.143	1896	1898	1900	rBV3	1902	1002	0.07%	0.008%
40	7.243	1918	1929	1955	rBV	692571	1219394	80.46%	9.350%
41	7.554	2017	2026	2045	rBV	126881	229463	15.14%	1.760%
42	7.905	2123	2135	2160	rBV	821140	1379361	91.01%	10.577%
43	8.024	2164	2172	2198	rVV	320690	546738	36.08%	4.192%
44	8.365	2276	2278	2282	rBV5	1928	1627	0.11%	0.012%
45	8.696	2380	2381	2385	rBV4	1023	506	0.03%	0.004%
46	8.744	2393	2396	2397	rBV3	1584	828	0.05%	0.006%
47	8.786	2399	2409	2433	rVV	735959	1192464	78.68%	9.144%
48	9.294	2565	2567	2568	rBV2	2300	863	0.06%	0.007%
49	9.381	2592	2594	2599	rBV5	1427	1426	0.09%	0.011%
50	9.599	2660	2662	2666	rBV4	1075	679	0.04%	0.005%
51	9.641	2674	2675	2679	rBV4	1453	983	0.06%	0.008%
52	9.664	2680	2682	2686	rVB5	1372	760	0.05%	0.006%
53	9.683	2686	2688	2689	rBV2	1285	502	0.03%	0.004%
54	9.799	2721	2724	2728	rBV4	2784	2646	0.17%	0.020%
55	9.869	2743	2746	2752	rVB8	1646	1817	0.12%	0.014%
56	9.895	2752	2754	2755	rBV2	1003	348	0.02%	0.003%
57	9.905	2755	2757	2759	rBV3	1126	520	0.03%	0.004%
58	9.934	2764	2766	2767	rBV2	675	276	0.02%	0.002%
59	10.152	2818	2834	2853	rBV	455811	727991	48.04%	5.582%
60	10.439	2921	2923	2925	rVB3	1776	723	0.05%	0.006%
61	10.458	2925	2929	2933	rBV6	2882	2320	0.15%	0.018%
62	10.632	2980	2983	2988	rBV5	1658	1832	0.12%	0.014%
63	10.677	2994	2997	3002	rBV7	1267	1061	0.07%	0.008%
64	10.943	3079	3080	3084	rVB4	1566	625	0.04%	0.005%
65	10.963	3084	3086	3090	rVB4	1337	606	0.04%	0.005%
66	11.088	3121	3125	3127	rBV3	1935	1804	0.12%	0.014%
67	11.188	3145	3156	3177	rBV	756597	1157993	76.41%	8.880%
68	11.400	3218	3222	3227	rVB8	2141	2005	0.13%	0.015%
69	11.422	3227	3229	3230	rBV3	871	452	0.03%	0.003%
70	11.506	3252	3255	3257	rBV4	1668	1153	0.08%	0.009%
71	11.561	3262	3272	3291	rVV	728789	1148987	75.81%	8.811%
72	11.898	3375	3377	3378	rBV	1121	450	0.03%	0.003%
73	12.001	3406	3409	3412	rBV4	1902	1281	0.08%	0.010%
74	12.117	3441	3445	3448	rBV5	1425	955	0.06%	0.007%
75	12.268	3489	3492	3494	rBV4	1808	1312	0.09%	0.010%
76	12.731	3633	3636	3643	rVB9	1803	1840	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032933.D
Acq On : 13 Nov 2023 15:51
Operator : SY/MD
Sample : 05326-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Title : VOC Analysis

77	12.760	3643	3645	3646	rBV2	1144	600	0.04%	0.005%
78	13.075	3739	3743	3745	rBV5	1181	1102	0.07%	0.008%
79	13.551	3888	3891	3896	rBV8	2157	2410	0.16%	0.018%
80	14.011	4032	4034	4035	rBV2	1610	522	0.03%	0.004%




Sum of corrected areas: 13041068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032933.D
Acq On : 13 Nov 2023 15:51
Operator : SY/MD
Sample : 05326-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

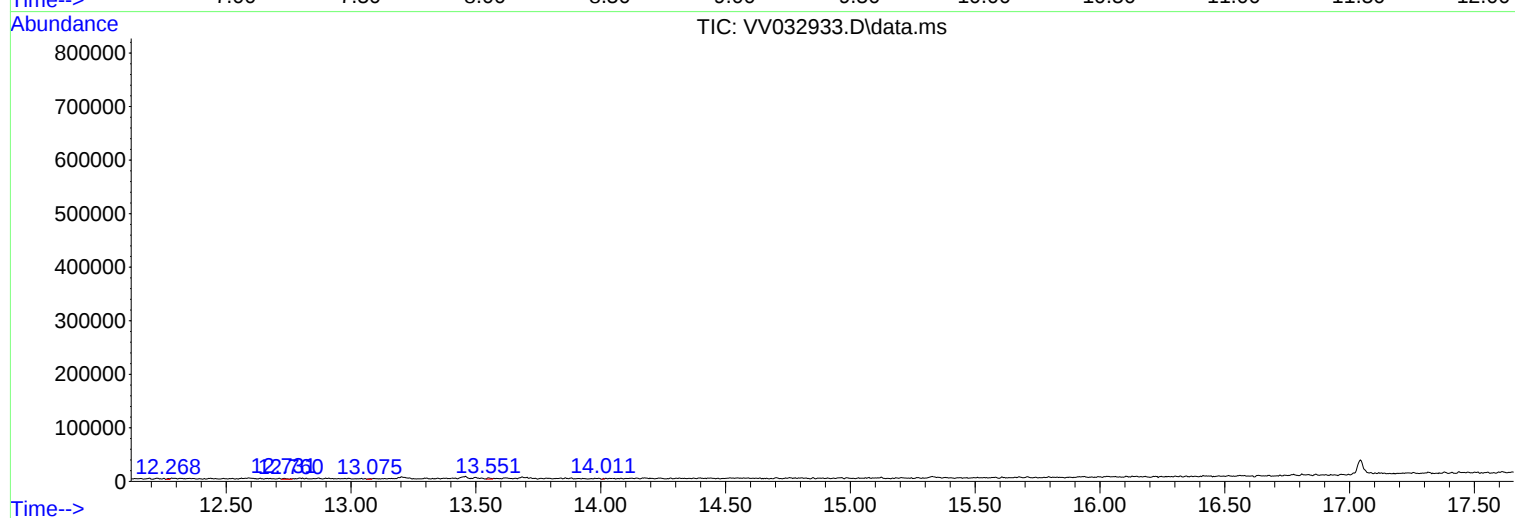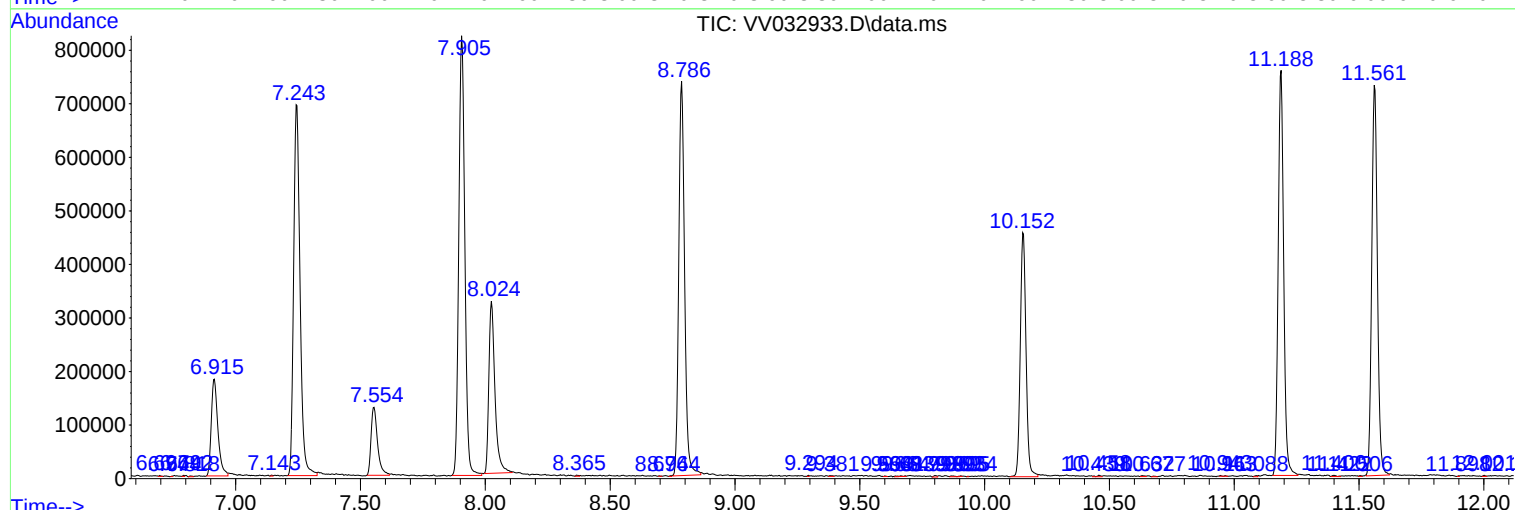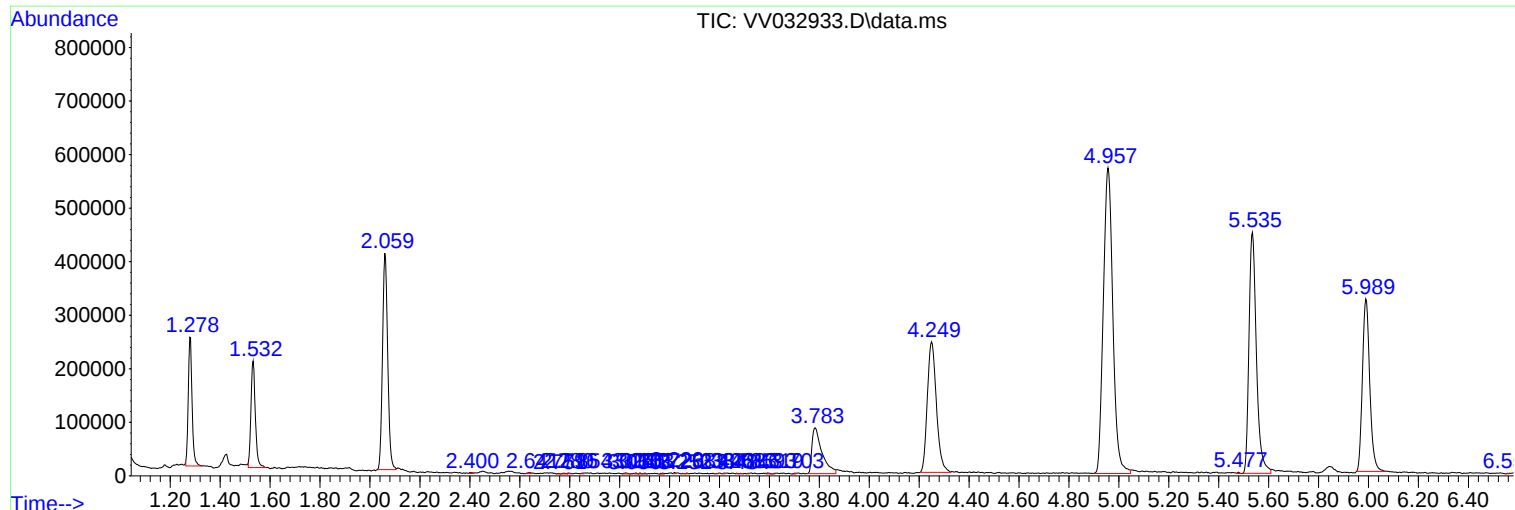

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032933.D
Acq On : 13 Nov 2023 15:51
Operator : SY/MD
Sample : 05326-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032933.D
Acq On : 13 Nov 2023 15:51
Operator : SY/MD
Sample : 05326-02DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------