

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032936.D
 Acq On : 13 Nov 2023 17:00
 Operator : SY/MD
 Sample : 05296-07
 Misc : 5.09gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	95	rVB	196361	291631	15.97%	2.112%
2	2.040	302	311	328	rVB	498741	720689	39.47%	5.219%
3	3.015	611	614	616	rBV4	1425	1102	0.06%	0.008%
4	3.066	629	630	631	rBV	841	293	0.02%	0.002%
5	3.159	657	659	662	rBV4	1382	1087	0.06%	0.008%
6	3.175	662	664	667	rVB4	1135	625	0.03%	0.005%
7	3.220	676	678	679	rBV2	1349	686	0.04%	0.005%
8	3.317	706	708	709	rBV2	1091	321	0.02%	0.002%
9	3.452	747	750	752	rBV4	2027	1133	0.06%	0.008%
10	3.532	773	775	778	rBV4	1453	1057	0.06%	0.008%
11	3.574	785	788	790	rBV3	1047	788	0.04%	0.006%
12	3.606	796	798	800	rBV3	927	596	0.03%	0.004%
13	3.632	803	806	811	rBV6	1800	1664	0.09%	0.012%
14	3.674	816	819	822	rBV5	1808	1224	0.07%	0.009%
15	3.693	822	825	826	rBV3	1102	643	0.04%	0.005%
16	3.722	832	834	835	rBV2	1690	769	0.04%	0.006%
17	3.767	843	848	852	rBV8	2231	2308	0.13%	0.017%
18	3.806	852	860	861	rBV2	59298	69595	3.81%	0.504%
19	4.249	985	998	1030	rVB2	277302	744975	40.80%	5.395%
20	4.445	1057	1059	1063	rVB5	2615	1386	0.08%	0.010%
21	4.465	1063	1065	1072	rBV8	2056	1771	0.10%	0.013%
22	4.716	1141	1143	1146	rBV4	1441	814	0.04%	0.006%
23	4.757	1155	1156	1163	rVB7	2033	2004	0.11%	0.015%
24	4.870	1190	1191	1196	rBV4	1434	831	0.05%	0.006%
25	4.892	1196	1198	1199	rBV2	1399	641	0.04%	0.005%
26	4.953	1202	1217	1241	rVV2	717206	1825886	100.00%	13.222%
27	5.391	1351	1353	1354	rBV2	1523	602	0.03%	0.004%
28	5.532	1386	1397	1427	rBV	528846	1156884	63.36%	8.377%
29	5.989	1527	1539	1565	rVB	372606	805425	44.11%	5.832%
30	6.416	1670	1672	1676	rBV4	1752	904	0.05%	0.007%
31	6.497	1694	1697	1698	rBV3	1555	882	0.05%	0.006%
32	6.510	1698	1701	1704	rVV3	1241	866	0.05%	0.006%
33	6.834	1798	1802	1803	rBV4	1360	947	0.05%	0.007%
34	6.915	1817	1827	1851	rBV	203522	418298	22.91%	3.029%
35	7.243	1918	1929	1951	rBV	835291	1505354	82.45%	10.901%
36	7.555	2017	2026	2047	rBV	138177	284468	15.58%	2.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032936.D
 Acq On : 13 Nov 2023 17:00
 Operator : SY/MD
 Sample : 05296-07
 Misc : 5.09gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	7.809	2102	2105	2109	rVB6	2169	1690	0.09%	0.012%
38	8.063	2167	2184	2206	rBV	210906	652369	35.73%	4.724%
39	8.539	2328	2332	2335	rBV5	2462	2003	0.11%	0.015%
40	8.657	2367	2369	2372	rBV4	1635	1124	0.06%	0.008%
41	8.789	2398	2410	2435	rBV	804312	1478921	81.00%	10.709%
42	9.288	2563	2565	2568	rBV3	2436	1566	0.09%	0.011%
43	9.448	2614	2615	2616	rBV	1093	394	0.02%	0.003%
44	9.677	2684	2686	2689	rBV4	1785	936	0.05%	0.007%
45	9.866	2742	2745	2746	rBV2	1382	674	0.04%	0.005%
46	9.931	2763	2765	2768	rBV4	1626	952	0.05%	0.007%
47	10.008	2786	2789	2793	rBV5	1444	1332	0.07%	0.010%
48	10.066	2799	2807	2816	rBV4	9132	15174	0.83%	0.110%
49	10.165	2824	2838	2855	rBV	490103	872321	47.78%	6.317%
50	10.474	2932	2934	2935	rBV2	1667	892	0.05%	0.006%
51	10.593	2969	2971	2974	rBV3	1884	788	0.04%	0.006%
52	10.934	3075	3077	3081	rVB5	1830	937	0.05%	0.007%
53	10.953	3081	3083	3086	rBV3	1891	1409	0.08%	0.010%
54	11.027	3098	3106	3109	rBV9	2323	2971	0.16%	0.022%
55	11.191	3146	3157	3178	rBV	952032	1486479	81.41%	10.764%
56	11.567	3263	3274	3293	rBV	905955	1426982	78.15%	10.333%
57	12.278	3493	3495	3496	rBV2	1273	349	0.02%	0.003%
58	12.426	3538	3541	3542	rBV3	1328	733	0.04%	0.005%
59	12.709	3620	3629	3630	rBV7	2148	2743	0.15%	0.020%
60	12.831	3663	3667	3671	rBV7	2685	2608	0.14%	0.019%
61	12.966	3706	3709	3710	rBV3	1430	943	0.05%	0.007%
62	13.124	3752	3758	3760	rBV7	2846	2421	0.13%	0.018%
63	14.439	4165	4167	4168	rBV2	2268	881	0.05%	0.006%




Sum of corrected areas: 13809741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032936.D
Acq On : 13 Nov 2023 17:00
Operator : SY/MD
Sample : 05296-07
Misc : 5.09gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

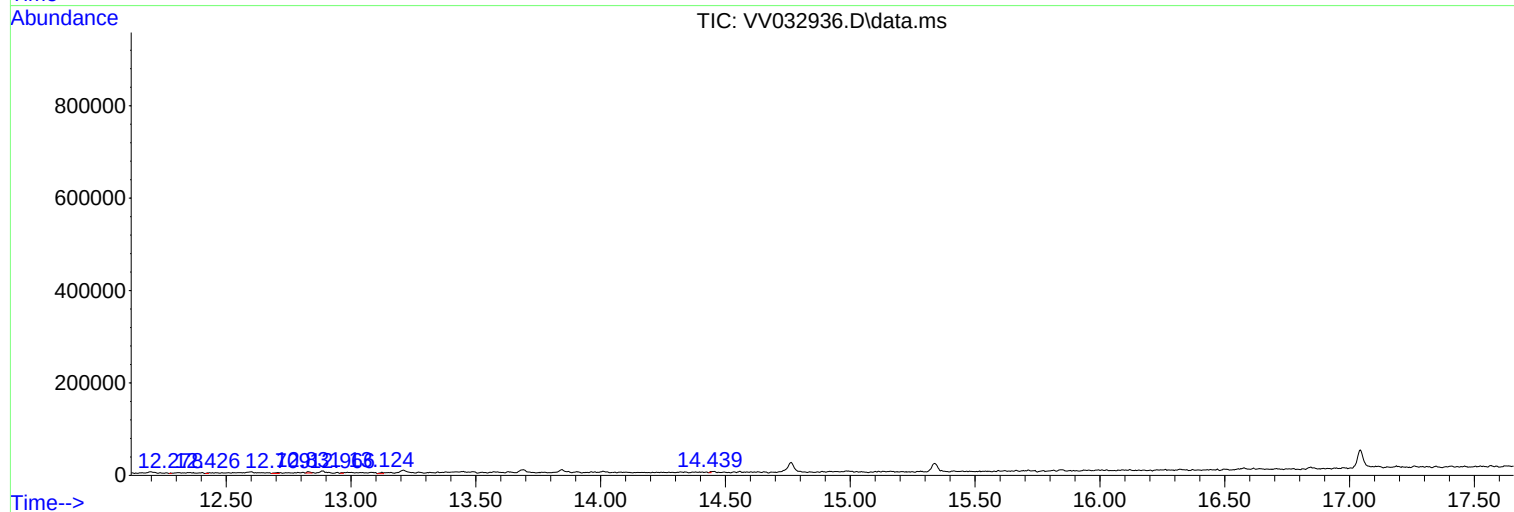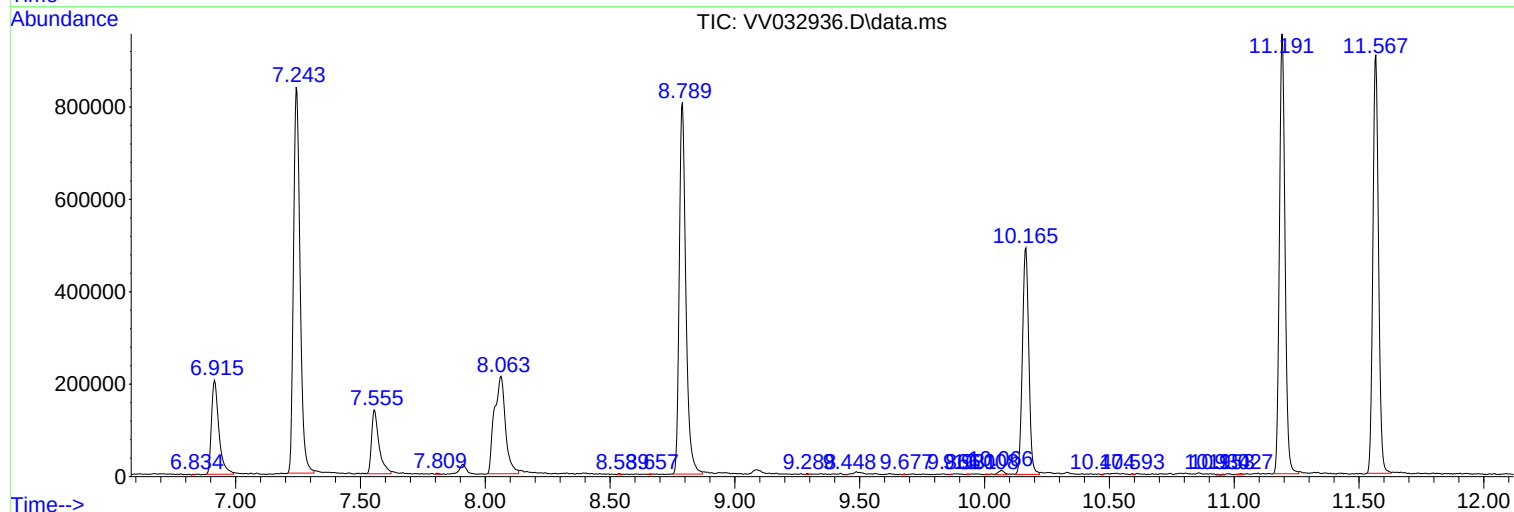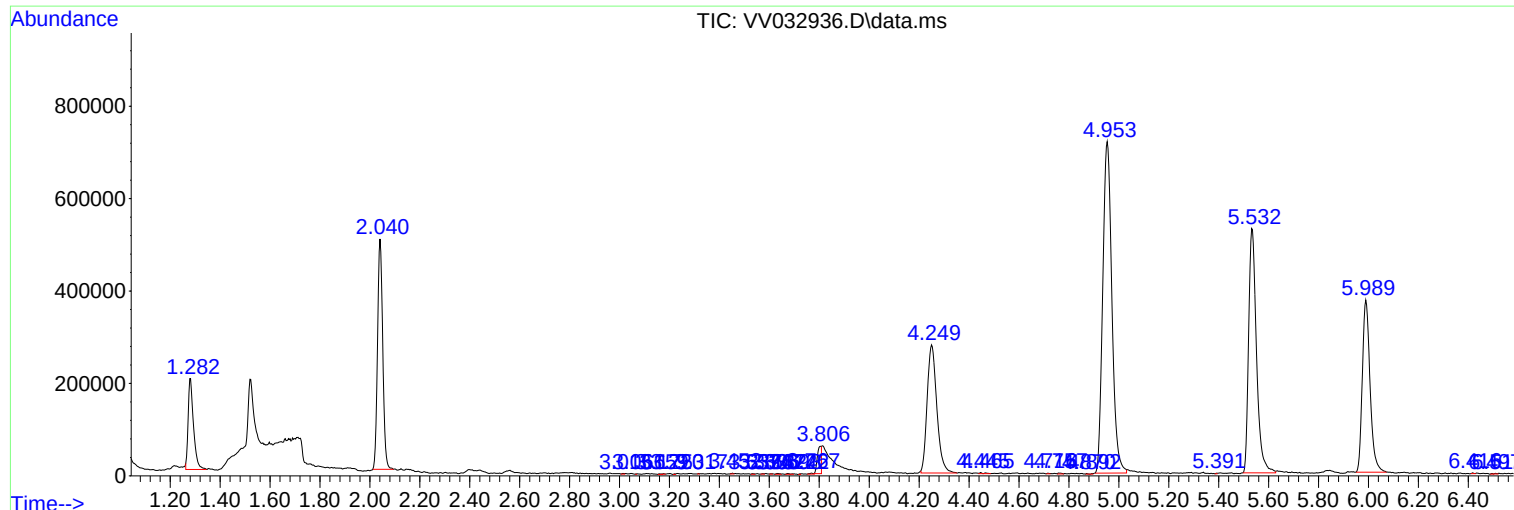

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032936.D
Acq On : 13 Nov 2023 17:00
Operator : SY/MD
Sample : 05296-07
Misc : 5.09gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032936.D
Acq On : 13 Nov 2023 17:00
Operator : SY/MD
Sample : 05296-07
Misc : 5.09gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc