

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032942.D
 Acq On : 13 Nov 2023 19:20
 Operator : SY/MD
 Sample : VIBLK245
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	240523	251475	16.63%	2.161%
2	1.532	147	153	170	rVB	204694	248104	16.41%	2.132%
3	2.060	308	317	333	rBV	407926	595279	39.38%	5.116%
4	2.333	400	402	404	rBV3	1234	626	0.04%	0.005%
5	2.388	417	419	424	rBV6	1626	1442	0.10%	0.012%
6	2.728	520	525	528	rBV7	1954	1730	0.11%	0.015%
7	2.773	533	539	540	rBV6	1637	1648	0.11%	0.014%
8	2.979	599	603	605	rBV4	1615	1478	0.10%	0.013%
9	3.008	609	612	616	rVV5	1623	1628	0.11%	0.014%
10	3.047	620	624	625	rBV4	1049	727	0.05%	0.006%
11	3.105	635	642	643	rBV6	1426	1638	0.11%	0.014%
12	3.182	664	666	668	rBV3	1913	1055	0.07%	0.009%
13	3.256	686	689	693	rVB5	2296	1607	0.11%	0.014%
14	3.278	693	696	698	rBV4	1272	741	0.05%	0.006%
15	3.490	758	762	768	rBV9	1622	1700	0.11%	0.015%
16	3.574	785	788	789	rBV3	1364	665	0.04%	0.006%
17	3.658	810	814	818	rBV4	1348	1232	0.08%	0.011%
18	3.738	834	839	840	rBV5	916	602	0.04%	0.005%
19	3.783	845	853	886	rVV	77116	214736	14.20%	1.845%
20	3.947	902	904	906	rBV3	2229	1115	0.07%	0.010%
21	4.249	984	998	1026	rVB	245397	622034	41.15%	5.346%
22	4.584	1100	1102	1104	rBV3	1248	655	0.04%	0.006%
23	4.957	1203	1218	1246	rBV2	573601	1511751	100.00%	12.992%
24	5.423	1361	1363	1365	rBV3	1263	626	0.04%	0.005%
25	5.535	1387	1398	1425	rBV	441457	903559	59.77%	7.765%
26	5.989	1527	1539	1569	rBV	333216	674312	44.60%	5.795%
27	6.461	1684	1686	1689	rBV4	1876	1059	0.07%	0.009%
28	6.641	1739	1742	1744	rBV3	1761	1264	0.08%	0.011%
29	6.706	1760	1762	1767	rBV6	1584	1527	0.10%	0.013%
30	6.744	1772	1774	1778	rVB5	1787	908	0.06%	0.008%
31	6.767	1778	1781	1782	rBV3	1670	708	0.05%	0.006%
32	6.802	1788	1792	1795	rVB4	1448	1295	0.09%	0.011%
33	6.831	1796	1801	1802	rBV3	1021	875	0.06%	0.008%
34	6.915	1817	1827	1848	rBV	179024	335965	22.22%	2.887%
35	7.169	1902	1906	1913	rBV9	2095	2594	0.17%	0.022%
36	7.243	1919	1929	1951	rBV	693948	1214468	80.34%	10.437%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111323\
 Data File : VW032942.D
 Acq On : 13 Nov 2023 19:20
 Operator : SY/MD
 Sample : VIBLK245
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	7.519	2013	2015	2016	rBV2	1820	693	0.05%	0.006%
38	7.551	2017	2025	2046	rVV	128625	228163	15.09%	1.961%
39	7.767	2090	2092	2094	rBV2	1625	1006	0.07%	0.009%
40	7.870	2120	2124	2126	rBV4	2969	2348	0.16%	0.020%
41	8.024	2163	2172	2195	rBV	287819	518150	34.27%	4.453%
42	8.584	2343	2346	2347	rBV3	1093	628	0.04%	0.005%
43	8.600	2349	2351	2354	rVB4	1621	840	0.06%	0.007%
44	8.625	2354	2359	2363	rBV5	2215	2441	0.16%	0.021%
45	8.674	2370	2374	2377	rBV5	1494	1272	0.08%	0.011%
46	8.709	2383	2385	2388	rBV4	1316	618	0.04%	0.005%
47	8.786	2395	2409	2433	rBV	726443	1191516	78.82%	10.240%
48	9.085	2499	2502	2505	rBV5	1730	1581	0.10%	0.014%
49	9.146	2519	2521	2524	rBV3	1544	741	0.05%	0.006%
50	9.233	2546	2548	2550	rBV3	1255	730	0.05%	0.006%
51	9.339	2579	2581	2584	rBV4	985	619	0.04%	0.005%
52	9.371	2587	2591	2595	rBV7	1511	1243	0.08%	0.011%
53	9.426	2605	2608	2611	rBV4	1727	858	0.06%	0.007%
54	9.519	2635	2637	2640	rBV4	1380	809	0.05%	0.007%
55	9.571	2648	2653	2657	rBV5	1575	1454	0.10%	0.012%
56	9.600	2657	2662	2663	rBV5	1785	1387	0.09%	0.012%
57	9.632	2668	2672	2678	rBV9	1046	1260	0.08%	0.011%
58	9.702	2691	2694	2698	rBV6	1835	1440	0.10%	0.012%
59	9.751	2707	2709	2712	rBV4	970	666	0.04%	0.006%
60	9.773	2714	2716	2719	rBV4	2033	1336	0.09%	0.011%
61	9.789	2719	2721	2724	rVB5	1544	667	0.04%	0.006%
62	9.815	2728	2729	2732	rBV3	1444	830	0.05%	0.007%
63	9.863	2741	2744	2745	rVB3	1274	634	0.04%	0.005%
64	9.944	2768	2769	2771	rBV2	1464	614	0.04%	0.005%
65	10.153	2823	2834	2855	rVV	453024	721662	47.74%	6.202%
66	10.394	2906	2909	2912	rVB5	1573	926	0.06%	0.008%
67	10.413	2912	2915	2916	rBV3	1122	663	0.04%	0.006%
68	10.561	2958	2961	2962	rBV3	1504	831	0.05%	0.007%
69	10.628	2979	2982	2984	rBV4	1136	651	0.04%	0.006%
70	10.699	3002	3004	3005	rBV2	1307	638	0.04%	0.005%
71	10.712	3005	3008	3010	rVB4	1444	849	0.06%	0.007%
72	10.837	3045	3047	3048	rBV2	1375	697	0.05%	0.006%
73	10.895	3064	3065	3069	rVB3	988	608	0.04%	0.005%
74	10.921	3069	3073	3075	rBV5	1231	829	0.05%	0.007%
75	11.011	3098	3101	3104	rBV4	1266	828	0.05%	0.007%
76	11.027	3104	3106	3108	rBV3	960	580	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032942.D
 Acq On : 13 Nov 2023 19:20
 Operator : SY/MD
 Sample : VIBLK245
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK245

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.098	3127	3128	3131	rBV3	1229	579	0.04%	0.005%
78	11.130	3136	3138	3141	rBV3	1408	970	0.06%	0.008%
79	11.188	3144	3156	3180	rBV	735567	1141457	75.51%	9.810%
80	11.435	3231	3233	3236	rVB4	1464	736	0.05%	0.006%
81	11.497	3249	3252	3254	rBV4	1761	1202	0.08%	0.010%
82	11.561	3261	3272	3294	rBV	740310	1158774	76.65%	9.959%
83	11.741	3326	3328	3332	rBV5	1600	1283	0.08%	0.011%
84	12.165	3458	3460	3465	rVB6	1424	848	0.06%	0.007%
85	12.223	3476	3478	3480	rBV3	1241	654	0.04%	0.006%
86	12.349	3514	3517	3518	rBV3	1166	587	0.04%	0.005%
87	12.400	3530	3533	3535	rBV3	1401	882	0.06%	0.008%
88	12.455	3547	3550	3554	rVB5	3037	1884	0.12%	0.016%
89	12.480	3554	3558	3560	rBV5	1827	1219	0.08%	0.010%
90	12.651	3607	3611	3614	rBV6	2380	2067	0.14%	0.018%
91	12.667	3614	3616	3621	rVV6	1255	1091	0.07%	0.009%
92	12.699	3623	3626	3628	rBV4	1146	710	0.05%	0.006%
93	12.783	3650	3652	3654	rBV3	1568	865	0.06%	0.007%
94	12.985	3712	3715	3718	rBV4	2101	1609	0.11%	0.014%
95	13.194	3777	3780	3781	rBV4	1828	870	0.06%	0.007%
96	13.625	3911	3914	3917	rBV4	1605	1095	0.07%	0.009%
97	13.686	3925	3933	3946	rBV4	8844	16921	1.12%	0.145%
98	13.815	3969	3973	3976	rBV6	992	883	0.06%	0.008%
99	14.078	4053	4055	4057	rBV3	1368	657	0.04%	0.006%
100	14.850	4293	4295	4296	rBV2	1714	808	0.05%	0.007%




Sum of corrected areas: 11635785

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032942.D
Acq On : 13 Nov 2023 19:20
Operator : SY/MD
Sample : VIBLK245
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

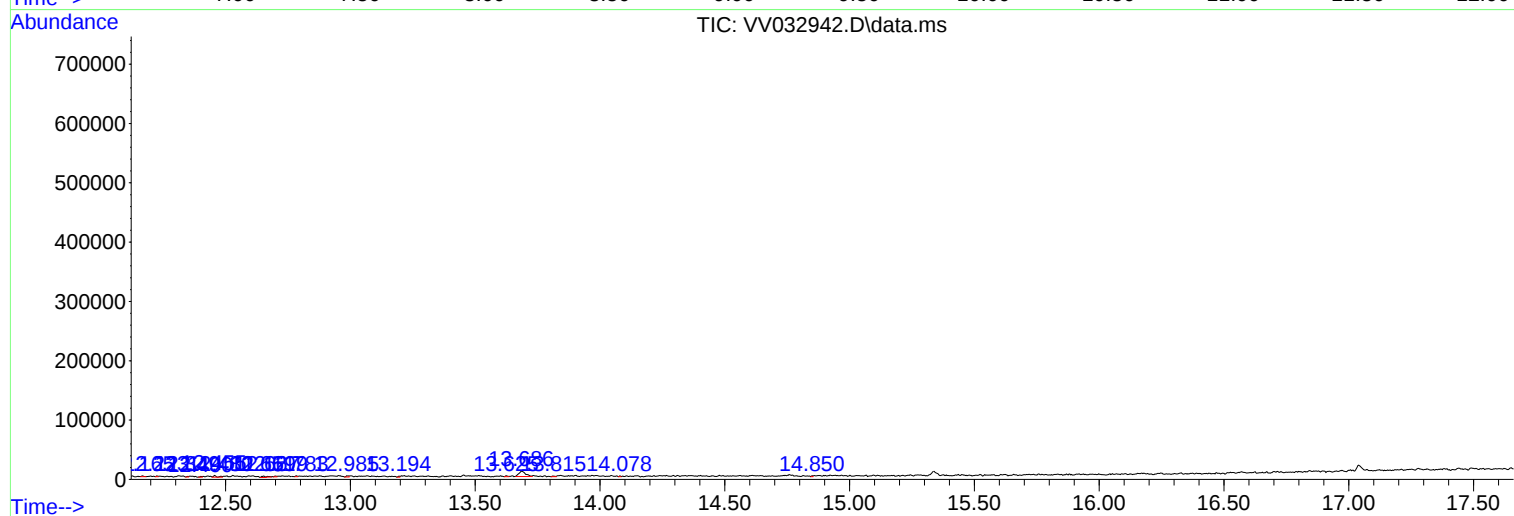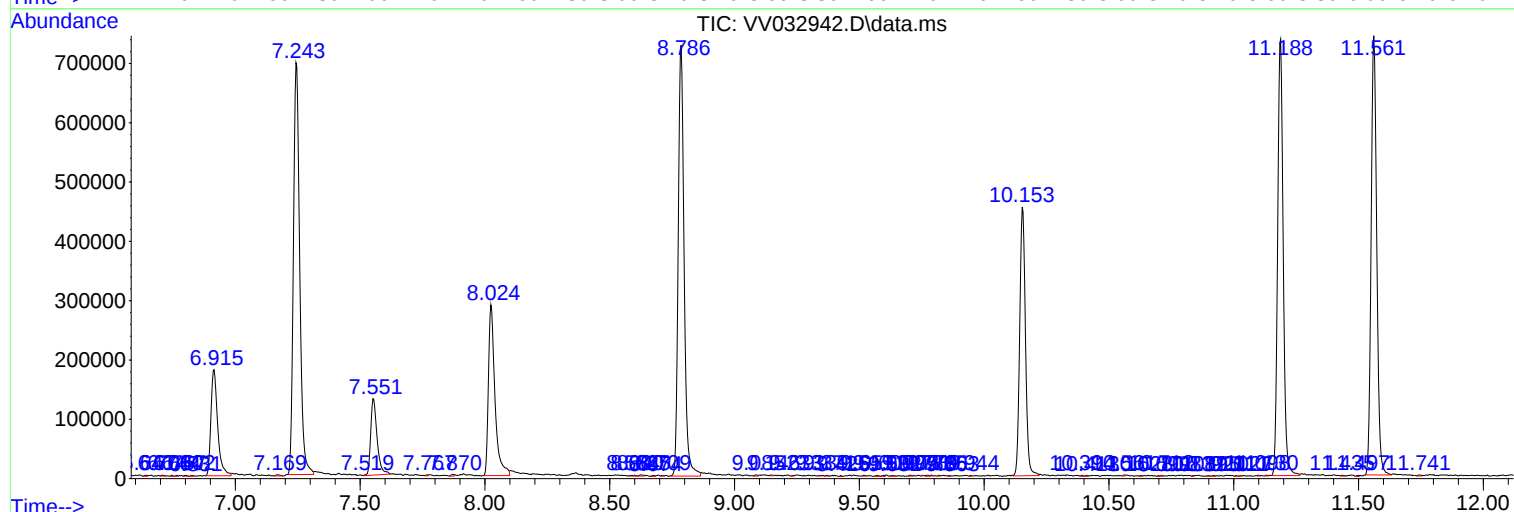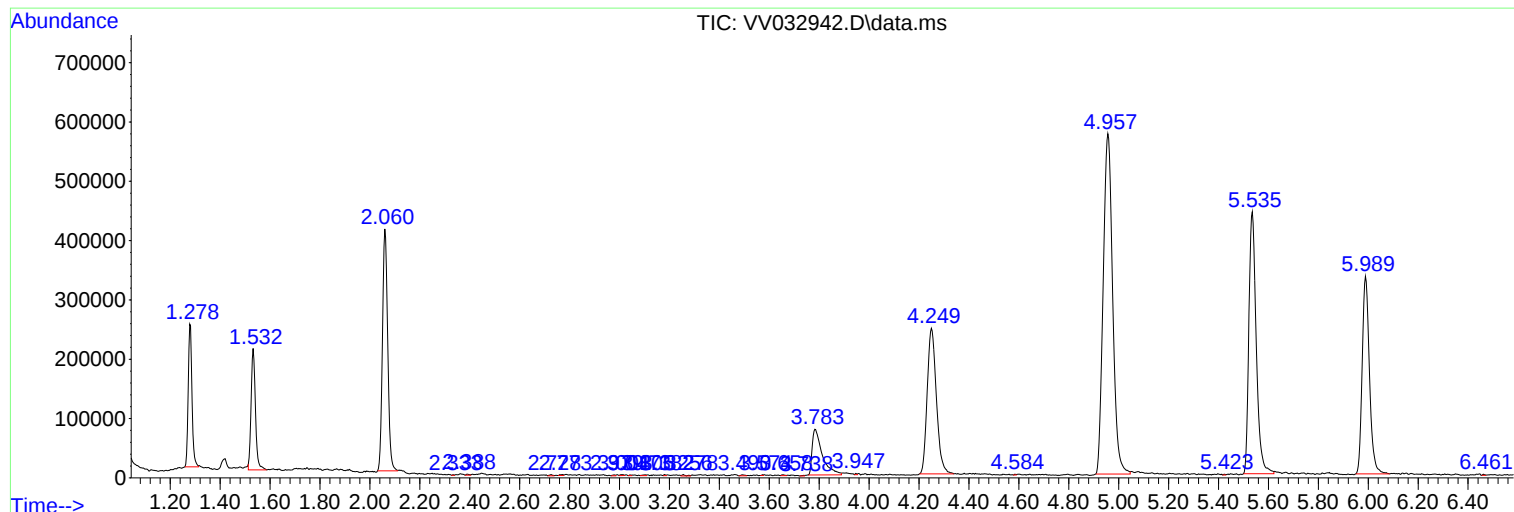

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032942.D
Acq On : 13 Nov 2023 19:20
Operator : SY/MD
Sample : VIBLK245
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032942.D
Acq On : 13 Nov 2023 19:20
Operator : SY/MD
Sample : VIBLK245
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc