

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032945.D
 Acq On : 13 Nov 2023 20:53
 Operator : SY/MD
 Sample : VV1113WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	257144	265137	15.86%	2.102%
2	1.532	147	153	166	rVB	216021	254960	15.25%	2.022%
3	2.060	308	317	333	rBV	435846	635982	38.04%	5.043%
4	2.400	421	423	427	rBV5	1291	744	0.04%	0.006%
5	2.757	532	534	538	rBV5	976	603	0.04%	0.005%
6	2.809	546	550	552	rBV5	1899	1325	0.08%	0.011%
7	2.854	561	564	567	rBV5	1161	791	0.05%	0.006%
8	2.915	581	583	584	rBV2	1424	674	0.04%	0.005%
9	2.963	595	598	601	rVB4	1853	1227	0.07%	0.010%
10	2.989	602	606	609	rBV6	1004	652	0.04%	0.005%
11	3.014	612	614	615	rBV2	1323	619	0.04%	0.005%
12	3.088	634	637	638	rVB2	1105	508	0.03%	0.004%
13	3.105	638	642	644	rBV5	2590	1597	0.10%	0.013%
14	3.121	644	647	651	rVV6	1385	1298	0.08%	0.010%
15	3.159	657	659	665	rBV7	1025	915	0.05%	0.007%
16	3.240	678	684	687	rBV7	1647	1528	0.09%	0.012%
17	3.281	694	697	702	rBV6	1800	1808	0.11%	0.014%
18	3.307	703	705	708	rVB4	1972	996	0.06%	0.008%
19	3.346	715	717	718	rBV2	1085	611	0.04%	0.005%
20	3.397	731	733	736	rVB4	1706	1037	0.06%	0.008%
21	3.432	741	744	747	rBV5	1495	886	0.05%	0.007%
22	3.468	752	755	756	rBV3	946	526	0.03%	0.004%
23	3.526	771	773	776	rVB4	1093	622	0.04%	0.005%
24	3.548	776	780	785	rBV8	1837	1668	0.10%	0.013%
25	3.593	791	794	795	rBV3	1342	700	0.04%	0.006%
26	3.661	810	815	820	rBV9	1922	1796	0.11%	0.014%
27	3.696	820	826	828	rBV6	2354	1971	0.12%	0.016%
28	3.783	844	853	874	rBV2	86966	231152	13.82%	1.833%
29	4.249	983	998	1021	rBV	266977	686754	41.07%	5.446%
30	4.567	1095	1097	1099	rBV2	1576	524	0.03%	0.004%
31	4.796	1166	1168	1169	rBV2	1305	520	0.03%	0.004%
32	4.957	1201	1218	1251	rBV2	630500	1672055	100.00%	13.259%
33	5.365	1343	1345	1347	rBV3	1517	623	0.04%	0.005%
34	5.487	1377	1383	1386	rBV8	1926	2484	0.15%	0.020%
35	5.535	1386	1398	1427	rVV	462808	948686	56.74%	7.523%
36	5.989	1526	1539	1557	rBV	362857	738027	44.14%	5.852%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032945.D
 Acq On : 13 Nov 2023 20:53
 Operator : SY/MD
 Sample : VV1113WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.381	1658	1661	1664	rBV5	1460	1239	0.07%	0.010%
38	6.432	1672	1677	1678	rBV5	2706	2061	0.12%	0.016%
39	6.744	1770	1774	1777	rBV5	1992	1971	0.12%	0.016%
40	6.812	1792	1795	1796	rBV3	1335	841	0.05%	0.007%
41	6.915	1817	1827	1845	rBV	194973	360332	21.55%	2.857%
42	7.243	1918	1929	1955	rBV	759520	1339036	80.08%	10.618%
43	7.554	2017	2026	2044	rBV	142721	248986	14.89%	1.974%
44	7.760	2088	2090	2091	rBV2	1796	816	0.05%	0.006%
45	7.812	2104	2106	2109	rBV4	1097	696	0.04%	0.006%
46	7.850	2115	2118	2120	rBV4	1768	1190	0.07%	0.009%
47	8.024	2161	2172	2196	rBV	325158	583736	34.91%	4.629%
48	8.458	2303	2307	2309	rBV5	1826	1275	0.08%	0.010%
49	8.506	2320	2322	2324	rBV3	1730	841	0.05%	0.007%
50	8.587	2344	2347	2350	rBV5	1639	960	0.06%	0.008%
51	8.706	2381	2384	2390	rVB7	1761	1316	0.08%	0.010%
52	8.786	2398	2409	2425	rBV	744614	1214495	72.63%	9.630%
53	9.349	2580	2584	2586	rBV5	1707	1509	0.09%	0.012%
54	9.484	2622	2626	2627	rBV3	3077	2000	0.12%	0.016%
55	9.638	2672	2674	2676	rBV3	1604	675	0.04%	0.005%
56	9.693	2686	2691	2696	rVB8	2109	2563	0.15%	0.020%
57	9.722	2696	2700	2706	rBV9	1797	1713	0.10%	0.014%
58	9.815	2725	2729	2730	rBV3	1972	1147	0.07%	0.009%
59	9.931	2761	2765	2767	rBV5	1331	906	0.05%	0.007%
60	9.995	2783	2785	2789	rVB4	2153	1687	0.10%	0.013%
61	10.024	2789	2794	2797	rBV6	1436	1471	0.09%	0.012%
62	10.059	2803	2805	2808	rVB3	1376	683	0.04%	0.005%
63	10.152	2822	2834	2850	rBV	495012	789053	47.19%	6.257%
64	10.397	2908	2910	2914	rBV5	1080	614	0.04%	0.005%
65	10.416	2914	2916	2920	rVB4	1787	1041	0.06%	0.008%
66	10.439	2920	2923	2926	rBV5	1398	794	0.05%	0.006%
67	10.461	2926	2930	2932	rBV5	1257	938	0.06%	0.007%
68	10.487	2932	2938	2941	rBV8	2774	3095	0.19%	0.025%
69	10.564	2958	2962	2966	rBV5	2709	2078	0.12%	0.016%
70	10.799	3031	3035	3039	rBV7	1815	1525	0.09%	0.012%
71	10.844	3044	3049	3050	rBV5	2107	1553	0.09%	0.012%
72	10.934	3076	3077	3080	rBV3	850	511	0.03%	0.004%
73	10.976	3087	3090	3095	rBV6	1590	1441	0.09%	0.011%
74	11.066	3112	3118	3119	rBV7	1320	1159	0.07%	0.009%
75	11.188	3144	3156	3177	rBV	768691	1203512	71.98%	9.543%
76	11.342	3201	3204	3207	rVB5	2540	1567	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032945.D
 Acq On : 13 Nov 2023 20:53
 Operator : SY/MD
 Sample : VV1113WBL03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

77	11.365	3207	3211	3213	rBV4	1765	1191	0.07%	0.009%
78	11.516	3256	3258	3260	rBV4	1357	816	0.05%	0.006%
79	11.561	3261	3272	3287	rVV	818615	1283372	76.75%	10.176%
80	11.722	3318	3322	3326	rBV7	1823	2008	0.12%	0.016%
81	11.931	3383	3387	3391	rBV8	2126	2160	0.13%	0.017%
82	11.969	3396	3399	3400	rBV3	1323	914	0.05%	0.007%
83	12.320	3502	3508	3509	rBV5	1616	1438	0.09%	0.011%
84	12.516	3567	3569	3573	rVB5	1791	1172	0.07%	0.009%
85	12.535	3573	3575	3577	rBV3	1504	875	0.05%	0.007%
86	12.586	3584	3591	3602	rVV3	5868	9552	0.57%	0.076%
87	12.654	3611	3612	3615	rBV3	1363	657	0.04%	0.005%
88	12.770	3643	3648	3651	rBV6	2596	2530	0.15%	0.020%
89	12.853	3672	3674	3677	rBV5	1063	785	0.05%	0.006%
90	12.956	3702	3706	3709	rVB4	1306	908	0.05%	0.007%
91	13.204	3775	3783	3790	rBV4	6585	11818	0.71%	0.094%
92	13.268	3799	3803	3805	rBV4	1667	1522	0.09%	0.012%
93	13.448	3851	3859	3871	rVB3	10154	19389	1.16%	0.154%
94	13.561	3892	3894	3897	rVB3	2131	1079	0.06%	0.009%
95	13.606	3904	3908	3913	rBV8	1849	1779	0.11%	0.014%
96	13.683	3925	3932	3946	rBV6	9420	17152	1.03%	0.136%
97	13.934	4008	4010	4013	rVB3	1281	565	0.03%	0.004%
98	14.271	4111	4115	4117	rBV4	1504	1199	0.07%	0.010%
99	14.361	4140	4143	4146	rBV5	1871	1574	0.09%	0.012%
100	14.644	4227	4231	4233	rBV4	1967	1652	0.10%	0.013%




Sum of corrected areas: 12611139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032945.D
Acq On : 13 Nov 2023 20:53
Operator : SY/MD
Sample : VV1113WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

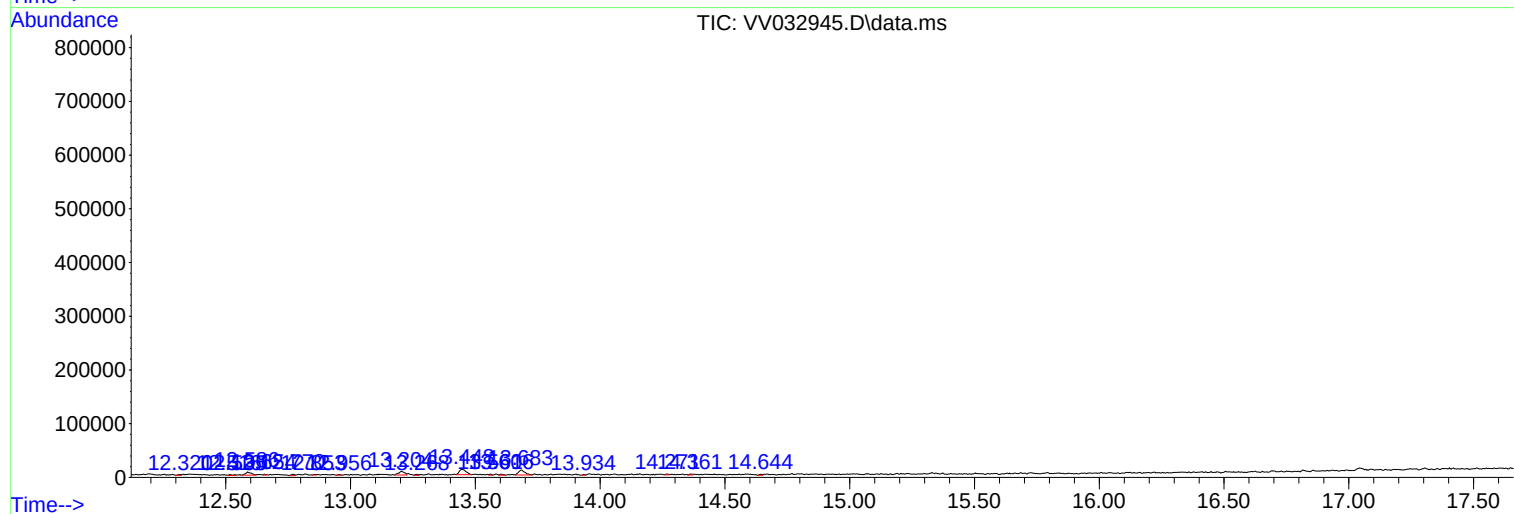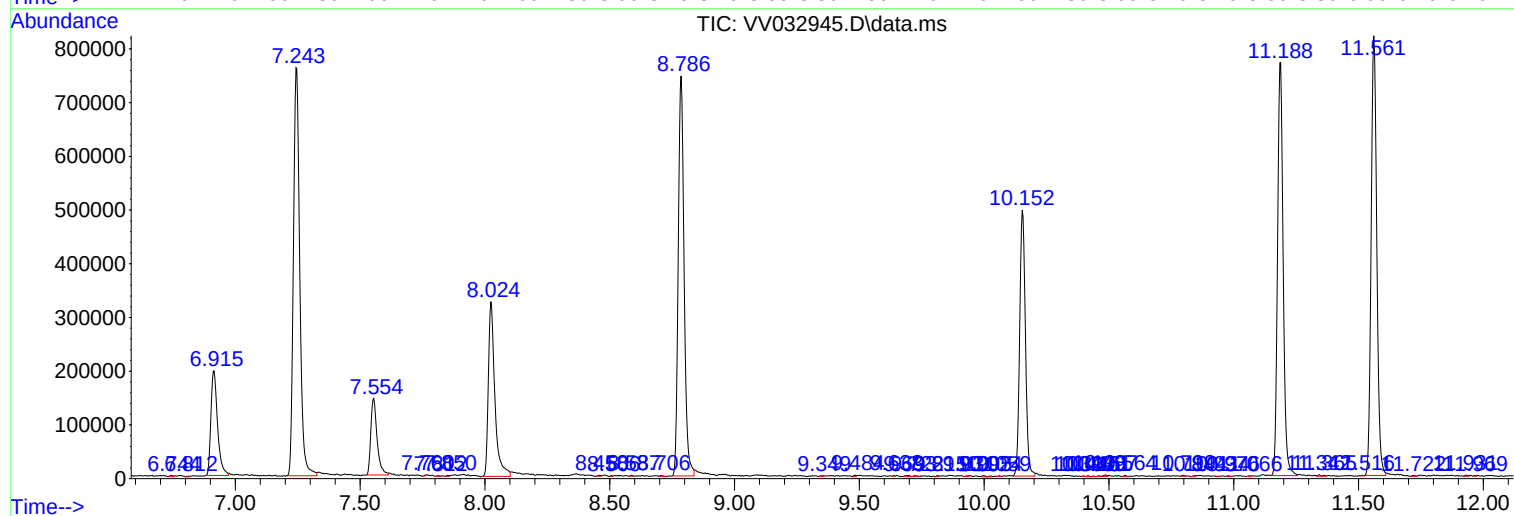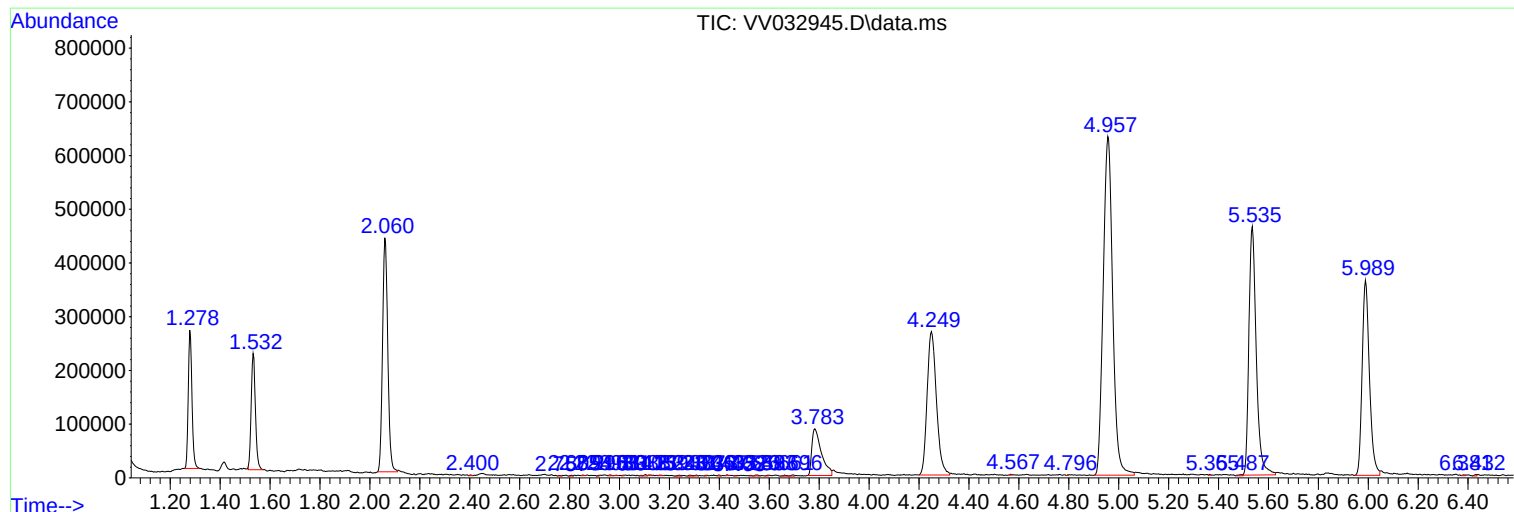

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032945.D
Acq On : 13 Nov 2023 20:53
Operator : SY/MD
Sample : VV1113WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032945.D
Acq On : 13 Nov 2023 20:53
Operator : SY/MD
Sample : VV1113WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK221

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------