

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032951.D
 Acq On : 13 Nov 2023 23:12
 Operator : SY/MD
 Sample : 05296-08 100X
 Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rBV	234953	243683	11.32%	1.492%
2	1.532	146	153	167	rVB	193849	231977	10.78%	1.420%
3	2.060	308	317	331	rBV	385858	557413	25.89%	3.412%
4	2.330	399	401	403	rBV3	1527	647	0.03%	0.004%
5	2.519	456	460	461	rBV4	1705	1045	0.05%	0.006%
6	2.664	501	505	508	rBV6	1701	1441	0.07%	0.009%
7	2.680	508	510	515	rVV5	1221	1051	0.05%	0.006%
8	2.754	531	533	536	rBV4	1239	819	0.04%	0.005%
9	2.786	541	543	545	rBV4	1394	797	0.04%	0.005%
10	2.822	553	554	555	rBV	808	195	0.01%	0.001%
11	2.867	567	568	569	rBV	1069	332	0.02%	0.002%
12	2.892	575	576	577	rBV	722	215	0.01%	0.001%
13	2.918	581	584	587	rVB3	1431	750	0.03%	0.005%
14	2.941	587	591	593	rBV4	1614	1372	0.06%	0.008%
15	2.963	596	598	601	rBV3	1399	881	0.04%	0.005%
16	3.011	609	613	615	rBV4	1111	765	0.04%	0.005%
17	3.063	627	629	635	rVB7	1915	1061	0.05%	0.006%
18	3.088	635	637	638	rBV2	995	347	0.02%	0.002%
19	3.117	642	646	647	rBV4	1445	755	0.04%	0.005%
20	3.150	654	656	659	rVB4	877	436	0.02%	0.003%
21	3.182	664	666	672	rVB6	1818	1545	0.07%	0.009%
22	3.214	672	676	679	rBV6	2116	2070	0.10%	0.013%
23	3.243	683	685	688	rVV4	1636	1218	0.06%	0.007%
24	3.275	691	695	697	rVB5	1133	801	0.04%	0.005%
25	3.301	699	703	704	rBV4	1035	708	0.03%	0.004%
26	3.323	708	710	711	rVB3	699	246	0.01%	0.002%
27	3.436	742	745	748	rBV4	740	651	0.03%	0.004%
28	3.461	750	753	756	rVV4	1138	805	0.04%	0.005%
29	3.561	783	784	789	rVB4	853	520	0.02%	0.003%
30	3.584	789	791	794	rBV4	1050	672	0.03%	0.004%
31	3.606	796	798	803	rVB6	1160	721	0.03%	0.004%
32	3.635	804	807	809	rBV4	1641	988	0.05%	0.006%
33	3.661	812	815	818	rVB5	1157	589	0.03%	0.004%
34	3.712	824	831	834	rBV8	1740	1734	0.08%	0.011%
35	3.731	834	837	838	rBV3	917	453	0.02%	0.003%
36	3.751	841	843	844	rBV2	1501	591	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032951.D
 Acq On : 13 Nov 2023 23:12
 Operator : SY/MD
 Sample : 05296-08 100X
 Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	3.783	845	853	888	rVV	78481	242206	11.25%	1.483%
38	4.249	984	998	1023	rBV	236493	608664	28.27%	3.726%
39	4.535	1085	1087	1089	rBV3	1160	549	0.03%	0.003%
40	4.648	1116	1122	1125	rBV7	2176	1966	0.09%	0.012%
41	4.690	1134	1135	1136	rBV	949	288	0.01%	0.002%
42	4.780	1162	1163	1164	rVB	1005	194	0.01%	0.001%
43	4.841	1180	1182	1186	rVB6	1513	896	0.04%	0.005%
44	4.957	1200	1218	1243	rBV2	558507	1485772	69.02%	9.095%
45	5.471	1376	1378	1380	rBV3	1274	664	0.03%	0.004%
46	5.532	1387	1397	1427	rBV	435627	891846	41.43%	5.460%
47	5.989	1524	1539	1562	rBV	325641	679164	31.55%	4.158%
48	6.297	1633	1635	1638	rBV4	1019	405	0.02%	0.002%
49	6.413	1669	1671	1673	rBV2	1222	734	0.03%	0.004%
50	6.484	1689	1693	1695	rBV4	2062	1732	0.08%	0.011%
51	6.593	1725	1727	1729	rBV3	1613	936	0.04%	0.006%
52	6.683	1750	1755	1757	rBV5	1566	1004	0.05%	0.006%
53	6.747	1773	1775	1776	rBV2	629	200	0.01%	0.001%
54	6.770	1779	1782	1784	rVB3	1495	708	0.03%	0.004%
55	6.786	1784	1787	1790	rBV6	1040	911	0.04%	0.006%
56	6.821	1796	1798	1803	rVB6	1699	949	0.04%	0.006%
57	6.850	1803	1807	1809	rBV5	2158	1711	0.08%	0.010%
58	6.915	1816	1827	1847	rBV2	178795	332602	15.45%	2.036%
59	7.243	1919	1929	1948	rBV	661842	1148907	53.37%	7.033%
60	7.554	2017	2026	2050	rBV2	126890	230251	10.70%	1.410%
61	7.677	2062	2064	2065	rBV2	1579	579	0.03%	0.004%
62	7.963	2149	2153	2154	rBV3	1916	1463	0.07%	0.009%
63	8.024	2163	2172	2194	rBV	279487	504948	23.46%	3.091%
64	8.667	2370	2372	2373	rBV2	897	351	0.02%	0.002%
65	8.786	2397	2409	2432	rBV	702722	1181307	54.87%	7.232%
66	8.950	2452	2460	2476	rVB	125020	196613	9.13%	1.204%
67	9.072	2487	2498	2523	rBV	1354550	2152802	100.00%	13.179%
68	9.477	2613	2624	2646	rBV	763540	1193218	55.43%	7.305%
69	9.956	2768	2773	2775	rBV5	1376	1007	0.05%	0.006%
70	9.995	2782	2785	2787	rBV4	1828	1065	0.05%	0.007%
71	10.152	2819	2834	2855	rBV	447252	713596	33.15%	4.368%
72	10.577	2962	2966	2968	rBV5	1536	1128	0.05%	0.007%
73	10.638	2982	2985	2988	rBV4	2598	1827	0.08%	0.011%
74	10.660	2990	2992	2994	rBV4	1718	800	0.04%	0.005%
75	10.677	2994	2997	3001	rVV5	3214	3214	0.15%	0.020%
76	10.857	3046	3053	3067	rVB4	13871	23011	1.07%	0.141%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032951.D
 Acq On : 13 Nov 2023 23:12
 Operator : SY/MD
 Sample : 05296-08 100X
 Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M

Title : VOC Analysis

77	10.931	3074	3076	3078	rBV4	1870	883	0.04%	0.005%
78	11.188	3145	3156	3176	rBV	762311	1293034	60.06%	7.916%
79	11.561	3262	3272	3294	rVB	746895	1214238	56.40%	7.433%
80	12.509	3558	3567	3583	rBV	20170	42123	1.96%	0.258%
81	13.143	3762	3764	3765	rBV2	1589	394	0.02%	0.002%
82	13.201	3771	3782	3801	rBV	508582	796662	37.01%	4.877%
83	13.683	3922	3932	3949	rVB	197860	317469	14.75%	1.943%




Sum of corrected areas: 16335285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032951.D
Acq On : 13 Nov 2023 23:12
Operator : SY/MD
Sample : 05296-08 100X
Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

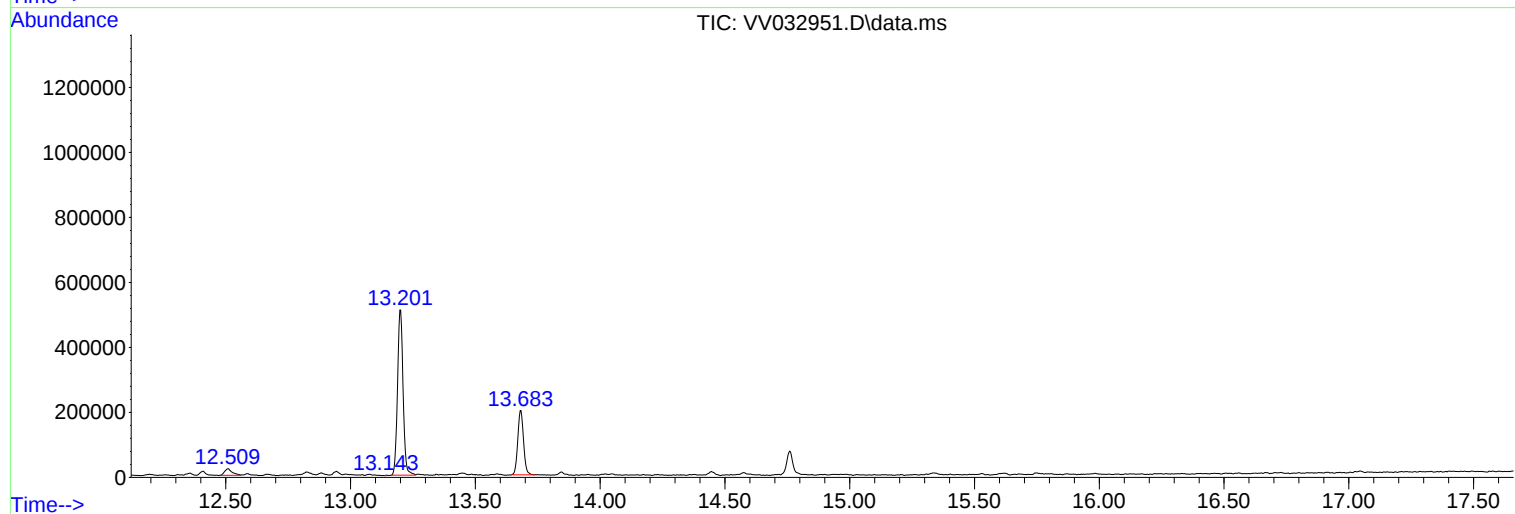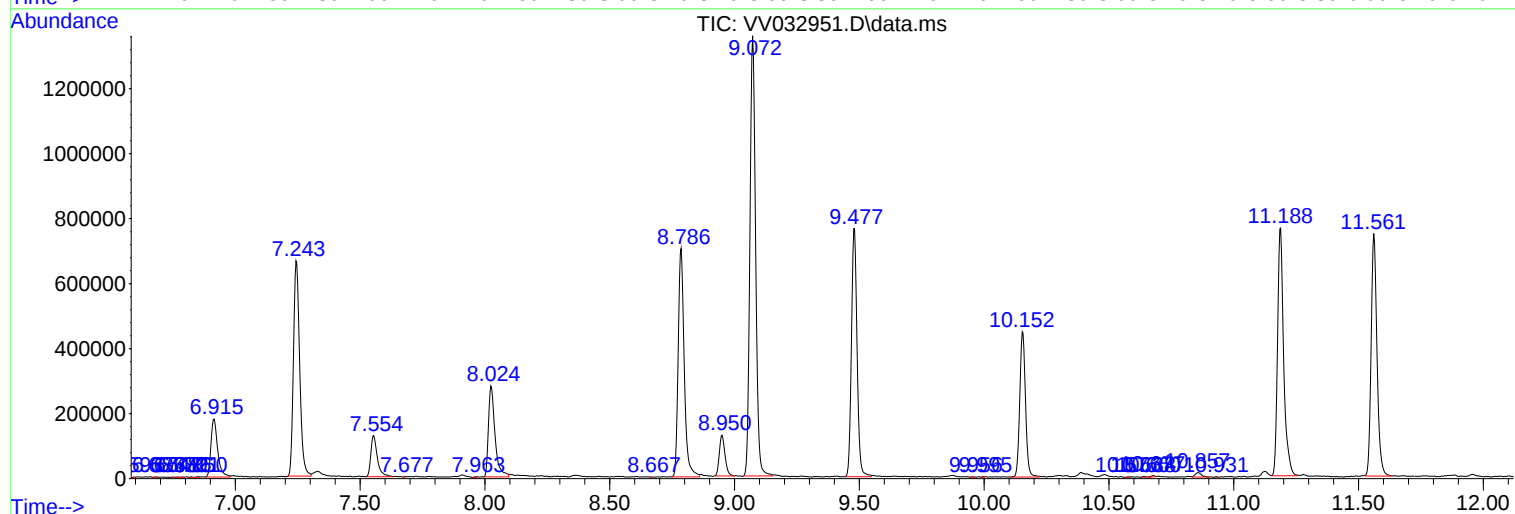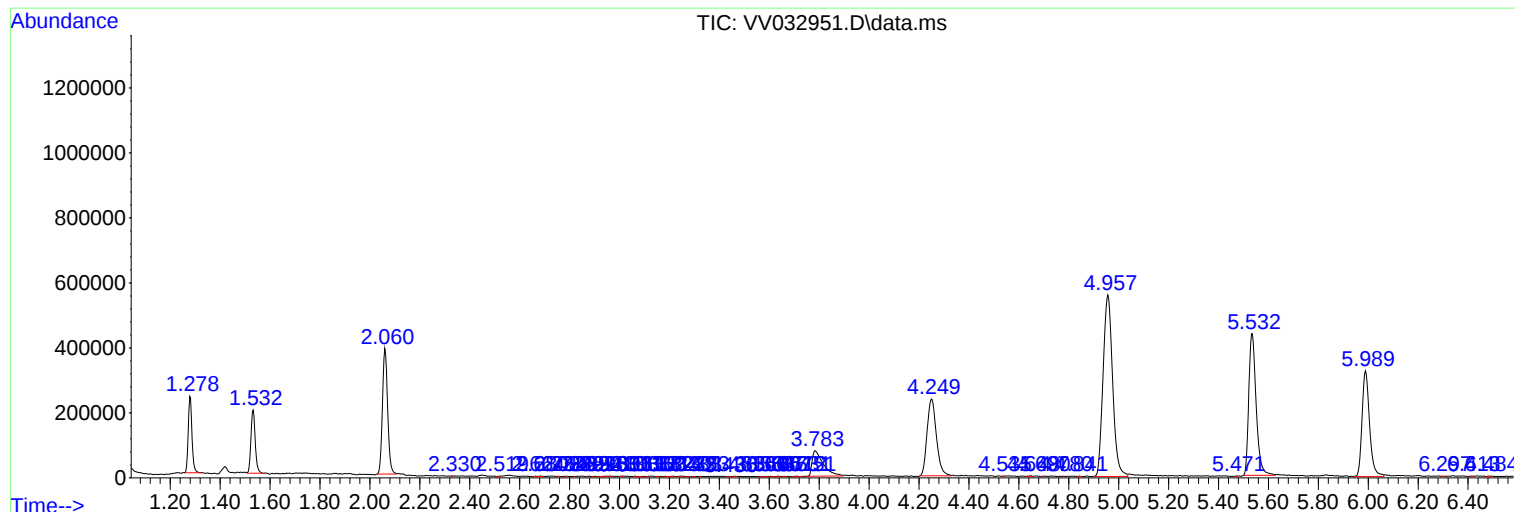

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032951.D
Acq On : 13 Nov 2023 23:12
Operator : SY/MD
Sample : 05296-08 100X
Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032951.D
Acq On : 13 Nov 2023 23:12
Operator : SY/MD
Sample : 05296-08 100X
Misc : 5.97gm/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3S1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------