

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032953.D
 Acq On : 13 Nov 2023 23:58
 Operator : SY/MD
 Sample : VIBLK246
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

Signal : TIC: VV032953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	88	rVB	200837	208430	14.46%	1.917%
2	1.532	147	153	170	rVB	178915	216086	14.99%	1.987%
3	2.060	308	317	332	rBV	338495	493873	34.26%	4.541%
4	2.812	549	551	553	rBV3	1667	1016	0.07%	0.009%
5	2.863	565	567	569	rVB3	1657	714	0.05%	0.007%
6	2.883	571	573	574	rBV2	1010	389	0.03%	0.004%
7	2.908	579	581	585	rBV5	1156	614	0.04%	0.006%
8	3.037	618	621	625	rVB6	2182	1738	0.12%	0.016%
9	3.069	625	631	638	rBV6	2122	3457	0.24%	0.032%
10	3.098	638	640	643	rBV4	1334	989	0.07%	0.009%
11	3.204	671	673	674	rBV2	771	245	0.02%	0.002%
12	3.275	691	695	696	rBV4	580	372	0.03%	0.003%
13	3.294	699	701	702	rBV2	1174	551	0.04%	0.005%
14	3.333	710	713	715	rBV4	1601	1144	0.08%	0.011%
15	3.346	715	717	720	rVV4	1359	909	0.06%	0.008%
16	3.378	726	727	730	rBV2	915	432	0.03%	0.004%
17	3.400	732	734	736	rVB2	1078	369	0.03%	0.003%
18	3.436	743	745	747	rBV3	979	369	0.03%	0.003%
19	3.523	770	772	775	rBV4	1586	922	0.06%	0.008%
20	3.609	794	799	801	rBV6	1511	1264	0.09%	0.012%
21	3.664	813	816	817	rBV3	1017	584	0.04%	0.005%
22	3.709	825	830	831	rBV5	1019	828	0.06%	0.008%
23	3.744	838	841	845	rBV4	2486	2015	0.14%	0.019%
24	3.783	845	853	877	rBV	79763	218452	15.15%	2.009%
25	4.153	966	968	971	rBV4	1268	638	0.04%	0.006%
26	4.249	985	998	1022	rVB	226540	577679	40.07%	5.312%
27	4.613	1109	1111	1114	rBV4	1622	988	0.07%	0.009%
28	4.847	1181	1184	1187	rBV5	925	693	0.05%	0.006%
29	4.957	1201	1218	1243	rBV2	540737	1441725	100.00%	13.257%
30	5.535	1387	1398	1423	rBV	386383	800923	55.55%	7.365%
31	5.989	1525	1539	1564	rBV	319644	664707	46.10%	6.112%
32	6.285	1627	1631	1634	rBV7	2505	2512	0.17%	0.023%
33	6.522	1703	1705	1708	rBV4	1518	1144	0.08%	0.011%
34	6.625	1734	1737	1739	rBV3	1830	1067	0.07%	0.010%
35	6.715	1763	1765	1766	rBV2	641	249	0.02%	0.002%
36	6.725	1766	1768	1773	rVV6	1928	1531	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
 Data File : VV032953.D
 Acq On : 13 Nov 2023 23:58
 Operator : SY/MD
 Sample : VIBLK246
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
 Title : VOC Analysis

37	6.828	1798	1800	1802	rVB2	1002	381	0.03%	0.004%
38	6.841	1802	1804	1808	rBV5	1215	941	0.07%	0.009%
39	6.860	1808	1810	1811	rBV2	934	346	0.02%	0.003%
40	6.911	1817	1826	1847	rBV	170956	318635	22.10%	2.930%
41	7.243	1919	1929	1950	rBV	650124	1135141	78.73%	10.438%
42	7.551	2017	2025	2047	rBV2	125594	223521	15.50%	2.055%
43	7.773	2092	2094	2097	rBV4	1551	1195	0.08%	0.011%
44	7.960	2149	2152	2155	rBV4	1795	1282	0.09%	0.012%
45	8.024	2163	2172	2200	rBV	308033	552426	38.32%	5.080%
46	8.651	2365	2367	2368	rBV2	1447	489	0.03%	0.004%
47	8.725	2388	2390	2392	rBV3	1204	607	0.04%	0.006%
48	8.786	2398	2409	2426	rBV	636333	1045592	72.52%	9.615%
49	9.172	2525	2529	2531	rBV5	1387	1063	0.07%	0.010%
50	9.484	2621	2626	2629	rBV6	3517	3505	0.24%	0.032%
51	9.554	2646	2648	2651	rBV3	1525	756	0.05%	0.007%
52	9.873	2743	2747	2752	rVB7	2163	2212	0.15%	0.020%
53	9.921	2760	2762	2765	rBV4	1714	1390	0.10%	0.013%
54	9.956	2771	2773	2778	rBV6	1237	1011	0.07%	0.009%
55	9.992	2783	2784	2785	rVB	1182	228	0.02%	0.002%
56	10.001	2785	2787	2790	rVB5	924	418	0.03%	0.004%
57	10.014	2790	2791	2792	rBV	736	182	0.01%	0.002%
58	10.024	2792	2794	2796	rVB2	1369	608	0.04%	0.006%
59	10.043	2796	2800	2801	rBV4	1821	1190	0.08%	0.011%
60	10.091	2812	2815	2818	rBV6	1692	977	0.07%	0.009%
61	10.153	2823	2834	2852	rVV	461504	722297	50.10%	6.642%
62	10.641	2984	2986	2988	rBV3	1084	632	0.04%	0.006%
63	10.693	2999	3002	3004	rBV3	2204	1276	0.09%	0.012%
64	10.757	3019	3022	3023	rBV3	1452	624	0.04%	0.006%
65	10.902	3065	3067	3068	rBV2	1190	479	0.03%	0.004%
66	10.956	3082	3084	3086	rBV3	1943	971	0.07%	0.009%
67	11.188	3145	3156	3174	rBV	657262	1036426	71.89%	9.530%
68	11.561	3261	3272	3296	rBV	716241	1128026	78.24%	10.373%
69	11.927	3384	3386	3389	rBV4	1282	698	0.05%	0.006%
70	12.101	3436	3440	3443	rBV6	1921	1618	0.11%	0.015%
71	12.230	3478	3480	3484	rVB4	1674	1044	0.07%	0.010%
72	12.439	3541	3545	3547	rBV5	1607	1555	0.11%	0.014%
73	12.522	3563	3571	3572	rBV5	2359	2793	0.19%	0.026%
74	12.696	3623	3625	3627	rBV3	1449	724	0.05%	0.007%
75	12.869	3677	3679	3680	rBV2	1628	578	0.04%	0.005%
76	13.358	3829	3831	3832	rBV2	1338	471	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032953.D
Acq On : 13 Nov 2023 23:58
Operator : SY/MD
Sample : VIBLK246
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M

Title : VOC Analysis

77	13.686	3927	3933	3942	rVB6	15162	23014	1.60%	0.212%
78	14.268	4110	4114	4117	rBV5	2034	1926	0.13%	0.018%
79	14.365	4139	4144	4147	rBV5	2159	2182	0.15%	0.020%
80	14.535	4193	4197	4199	rBV5	2593	1962	0.14%	0.018%
81	15.069	4360	4363	4367	rBV5	2436	1975	0.14%	0.018%




Sum of corrected areas: 10874985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032953.D
Acq On : 13 Nov 2023 23:58
Operator : SY/MD
Sample : VIBLK246
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

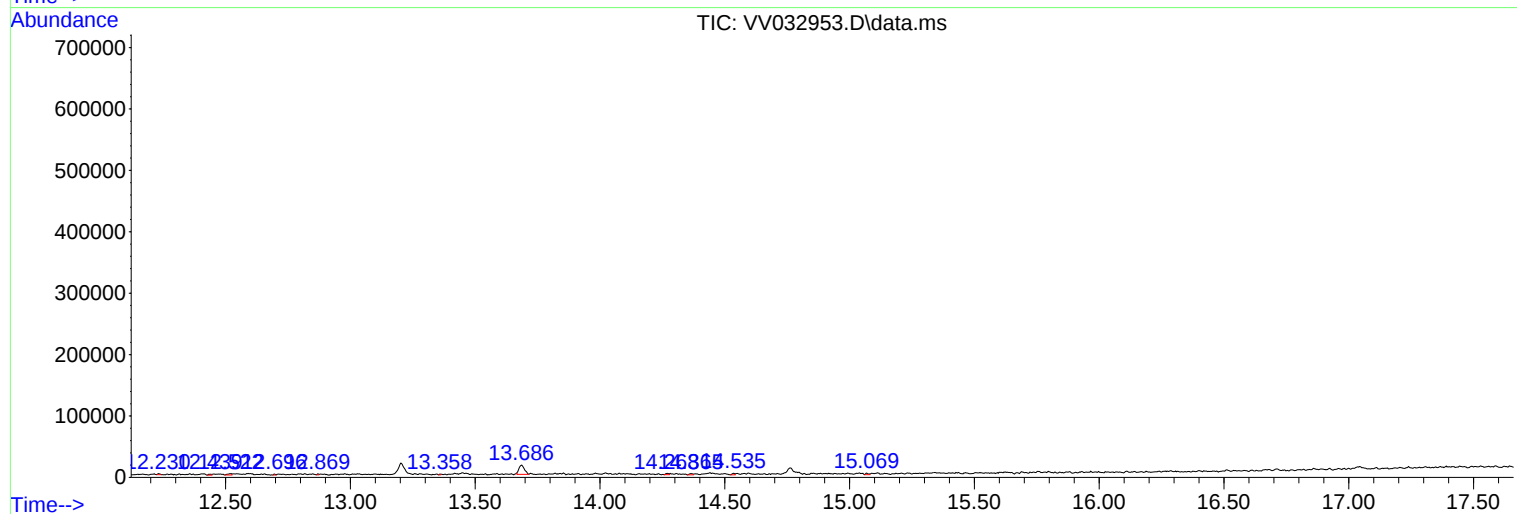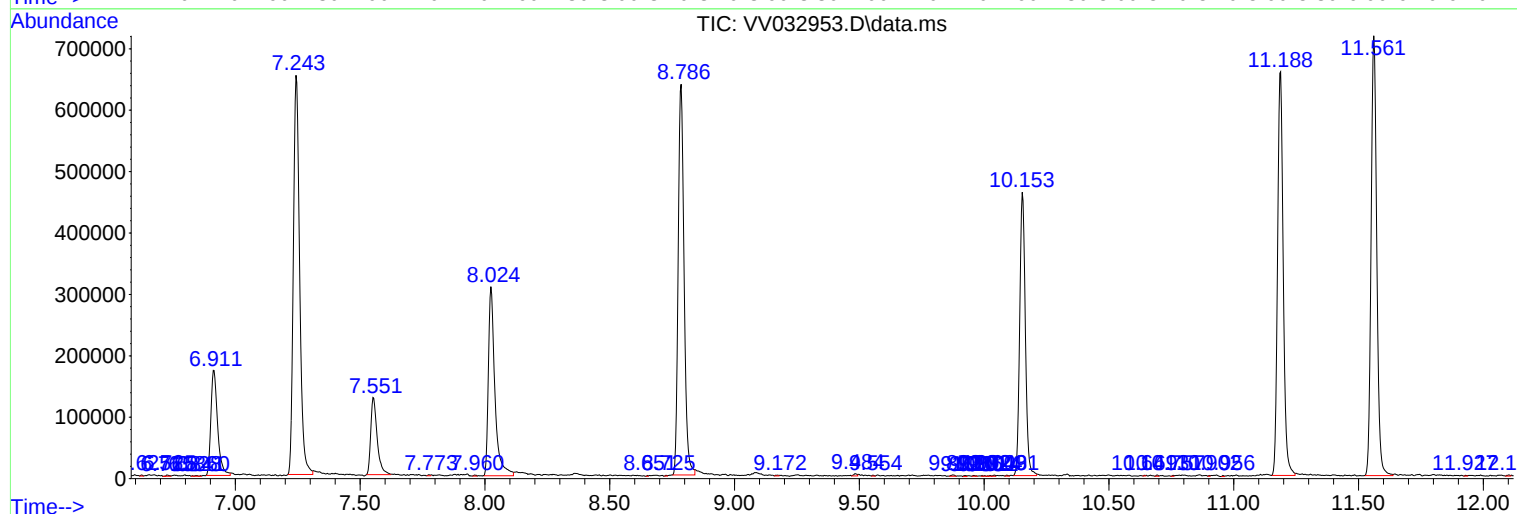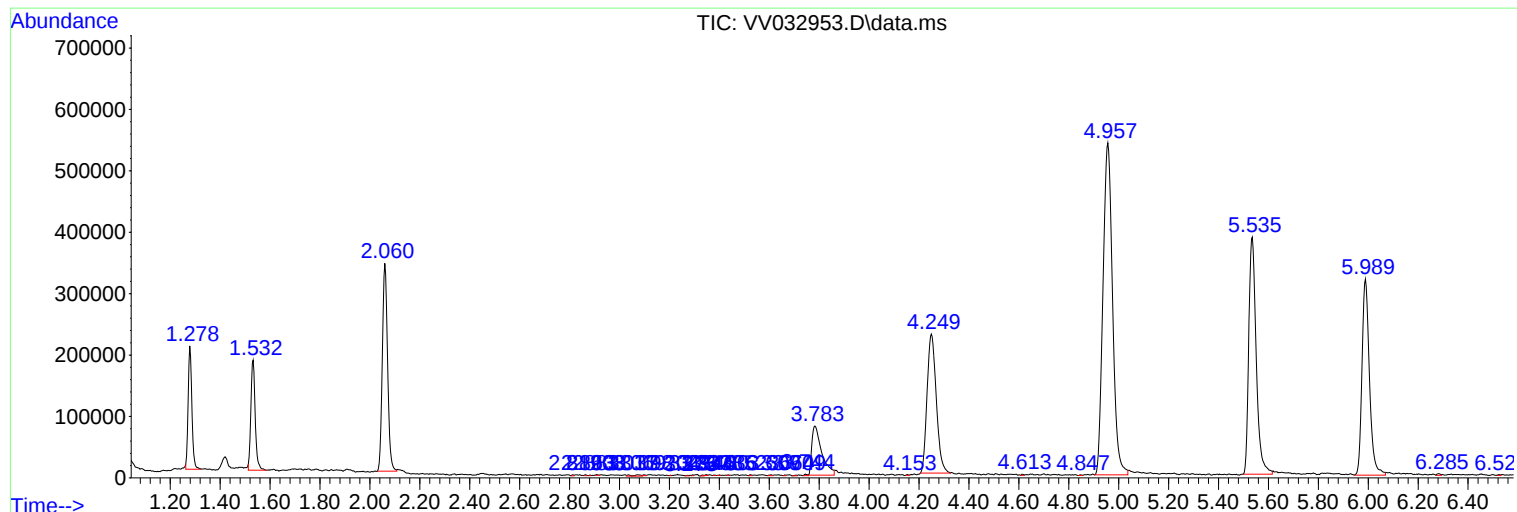

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032953.D
Acq On : 13 Nov 2023 23:58
Operator : SY/MD
Sample : VIBLK246
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032953.D
Acq On : 13 Nov 2023 23:58
Operator : SY/MD
Sample : VIBLK246
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------