
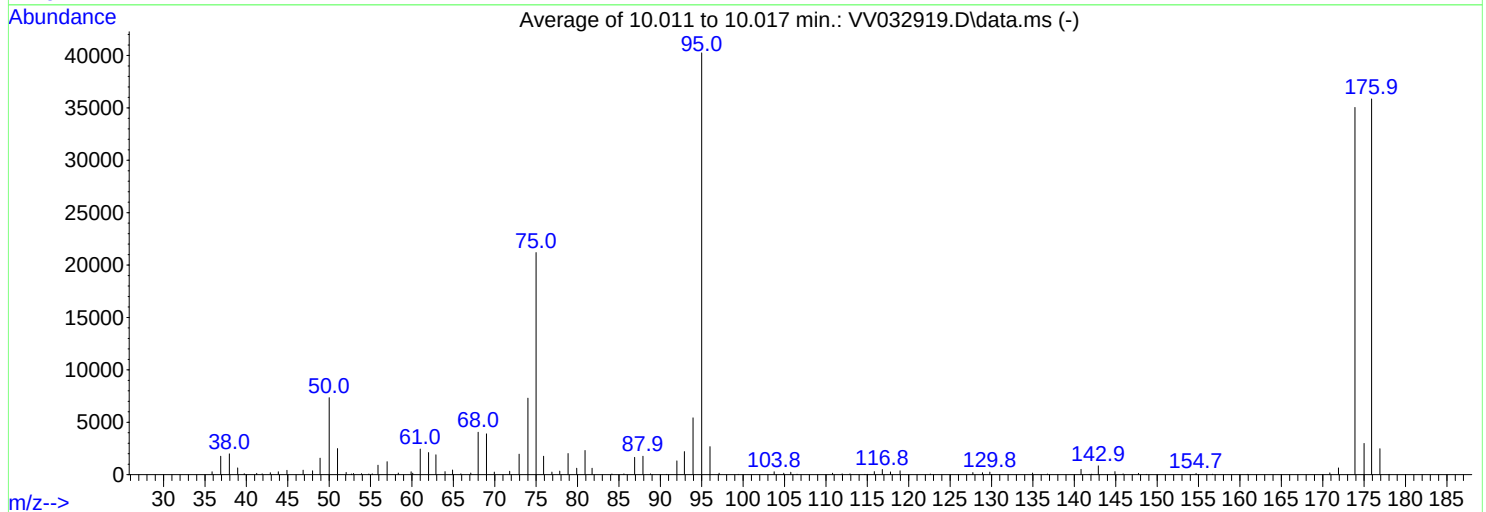


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111323\
Data File : VV032919.D
Acq On : 13 Nov 2023 09:26
Operator : SY/MD
Sample : BFB231
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB231

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111323WMA.M
Title : VOC Analysis
Last Update : Mon Nov 20 01:19:10 2023

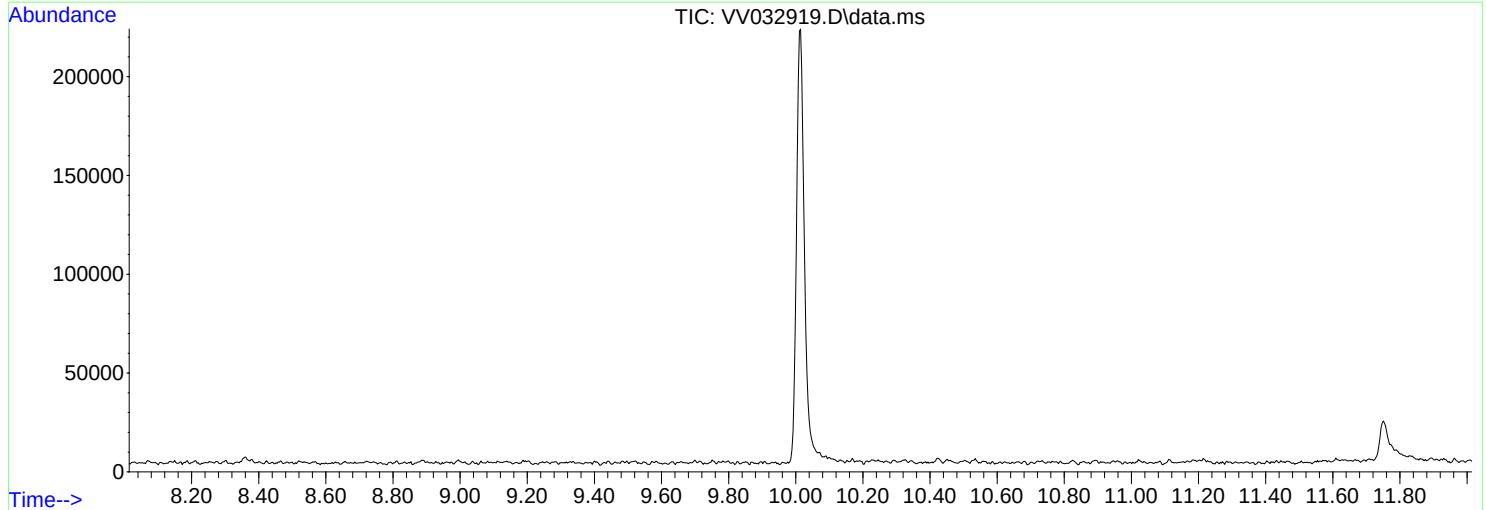

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	7351	PASS
75	95	30	80	52.7	21195	PASS
95	95	100	100	100.0	40253	PASS
96	95	5	9	6.7	2679	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.0	35040	PASS
175	174	5	9	8.5	2975	PASS
176	174	95	105	102.3	35851	PASS
177	176	5	10	6.9	2478	PASS

m/z	Abundance
35.10	121.0
35.80	148.0
36.80	170.0
37.90	137.0
38.80	268.0
39.80	247.0
40.70	234.0
42.00	154.0
43.80	541.0
44.90	152.0
45.70	173.0
46.50	117.0
51.20	108.0
52.40	118.0
54.50	126.0
55.20	131.0
57.30	106.0
58.00	133.0
59.40	118.0
68.20	157.0
69.00	104.0
70.00	103.0
76.50	117.0
76.90	133.0
79.10	112.0
86.00	121.0
89.90	111.0
90.70	102.0
94.60	103.0
98.50	111.0
120.40	106.0
139.30	112.0
198.10	105.0
206.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	446.0
37.00	2090.0
38.00	2246.0
39.00	916.0
39.70	343.0
40.80	135.0
41.20	144.0
41.90	190.0
42.90	200.0
43.90	865.0
45.00	508.0
45.70	126.0
46.90	429.0
48.00	341.0
48.90	1373.0
50.00	7607.0
51.00	2514.0
52.00	225.0
52.70	165.0
53.90	166.0
55.20	216.0
55.90	867.0
57.00	1210.0
58.40	124.0
59.90	372.0
61.00	2650.0
62.00	2288.0
62.90	2030.0
64.10	277.0
64.90	448.0
65.90	137.0
67.10	199.0
68.00	4310.0
69.00	4101.0
70.00	307.0
71.80	277.0
73.00	2040.0
74.00	7807.0
75.00	22152.0
75.90	1803.0
76.90	413.0
77.90	387.0
78.80	2044.0
79.90	554.0
80.90	2376.0
81.80	642.0
84.20	101.0
85.60	116.0
86.90	1612.0
87.90	1874.0
90.80	228.0
92.00	1260.0
92.90	2204.0
94.00	5519.0
95.00	41400.0
96.00	2700.0
97.10	146.0
99.40	103.0
103.70	248.0
104.90	130.0
105.80	293.0
110.80	142.0
111.90	137.0
112.90	118.0
115.80	308.0
116.80	445.0
117.80	237.0
119.00	389.0
122.60	106.0
127.70	237.0
128.90	207.0
129.80	208.0
134.90	174.0
136.80	105.0
140.80	488.0
142.10	129.0
142.90	863.0
144.90	277.0
145.90	136.0
147.70	125.0
148.70	114.0
154.70	131.0
160.90	107.0
170.90	136.0
171.80	620.0
173.90	36016.0
175.00	3102.0
175.90	36152.0
176.90	2691.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	441.0
37.00	1970.0
38.00	2231.0
39.00	953.0
39.80	356.0
40.70	146.0
41.20	101.0
41.90	263.0
42.90	194.0
43.90	844.0
44.90	588.0
45.70	130.0
46.90	423.0
48.00	390.0
48.90	1632.0
50.00	7648.0
51.00	2692.0
52.00	223.0
52.90	152.0
53.90	119.0
55.20	243.0
55.90	942.0
57.00	1296.0
58.30	148.0
60.10	428.0
61.00	2522.0
62.00	2171.0
62.90	1976.0
64.00	291.0
64.90	432.0
65.90	115.0
67.10	159.0
68.00	4386.0
69.00	4093.0
70.00	350.0
71.80	329.0
73.00	1941.0
74.00	7496.0
75.00	21984.0
75.90	1819.0
76.90	392.0
77.90	370.0
78.90	2097.0
79.90	617.0
80.90	2370.0
81.70	615.0
84.10	101.0
85.60	102.0
86.90	1695.0
87.90	1829.0
88.80	112.0
90.80	196.0
92.00	1389.0
92.90	2295.0
93.90	5451.0
95.00	41656.0
96.00	2754.0
97.10	139.0
103.80	289.0
104.90	139.0
105.70	208.0
110.80	147.0
112.00	109.0
112.90	127.0
114.70	102.0
115.90	283.0
116.80	516.0
117.80	267.0
119.00	379.0
122.60	101.0
127.70	197.0
128.90	189.0
129.80	264.0
134.90	168.0
140.80	520.0
142.90	871.0
144.90	319.0
145.90	115.0
147.80	130.0
154.70	136.0
170.80	178.0
171.90	627.0
173.90	36072.0
175.00	3078.0
175.90	37200.0
176.90	2551.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231

m/z	Abundance
35.90	397.0
36.90	1702.0
38.00	1887.0
39.00	863.0
39.80	302.0
40.80	171.0
41.30	102.0
41.90	251.0
42.90	164.0
43.90	742.0
44.90	621.0
45.80	131.0
46.80	416.0
48.00	384.0
48.90	1705.0
50.00	6798.0
51.00	2594.0
52.10	211.0
53.00	194.0
54.80	208.0
55.20	187.0
55.90	919.0
57.00	1191.0
58.30	165.0
59.90	476.0
61.00	2153.0
62.00	1855.0
62.90	1684.0
63.90	313.0
64.90	464.0
67.10	116.0
68.00	3918.0
69.00	3808.0
69.90	401.0
71.80	364.0
72.90	1885.0
74.00	6586.0
75.00	19448.0
75.90	1639.0
76.90	321.0
77.80	274.0
78.90	1911.0
79.90	651.0
80.90	2159.0
81.70	556.0
85.80	116.0
86.90	1634.0
87.90	1581.0
88.80	121.0
92.00	1313.0
92.90	2082.0
93.90	5285.0
95.00	37704.0
96.00	2582.0
97.10	140.0
103.80	307.0
104.90	143.0
105.70	204.0
106.50	121.0
110.80	112.0
115.00	105.0
115.90	263.0
116.80	503.0
117.80	265.0
118.90	347.0
127.80	180.0
128.90	174.0
129.80	254.0
135.00	136.0
136.70	102.0
140.80	526.0
141.80	106.0
142.90	804.0
144.90	284.0
147.80	118.0
154.70	120.0
156.70	157.0
170.90	192.0
172.00	665.0
173.90	33032.0
175.00	2746.0
175.90	34200.0
176.90	2191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB231