
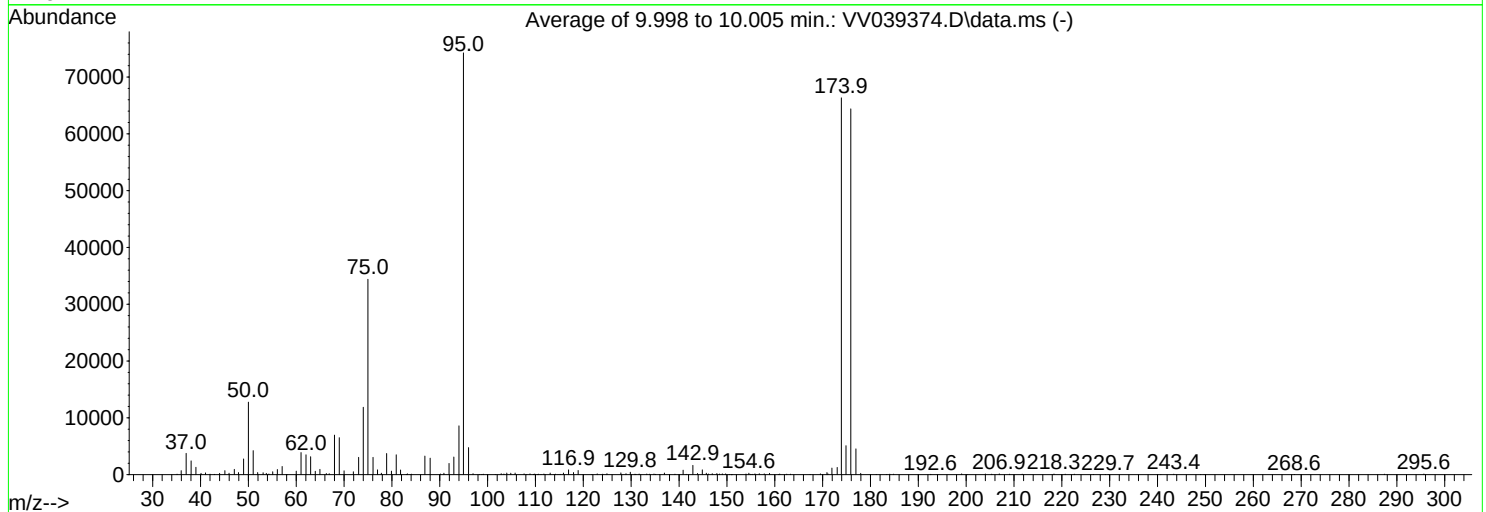


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111325\
Data File : VV039374.D
Acq On : 13 Nov 2025 09:02
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V111125W.M
Title : SW846 8260
Last Update : Wed Nov 12 01:49:22 2025

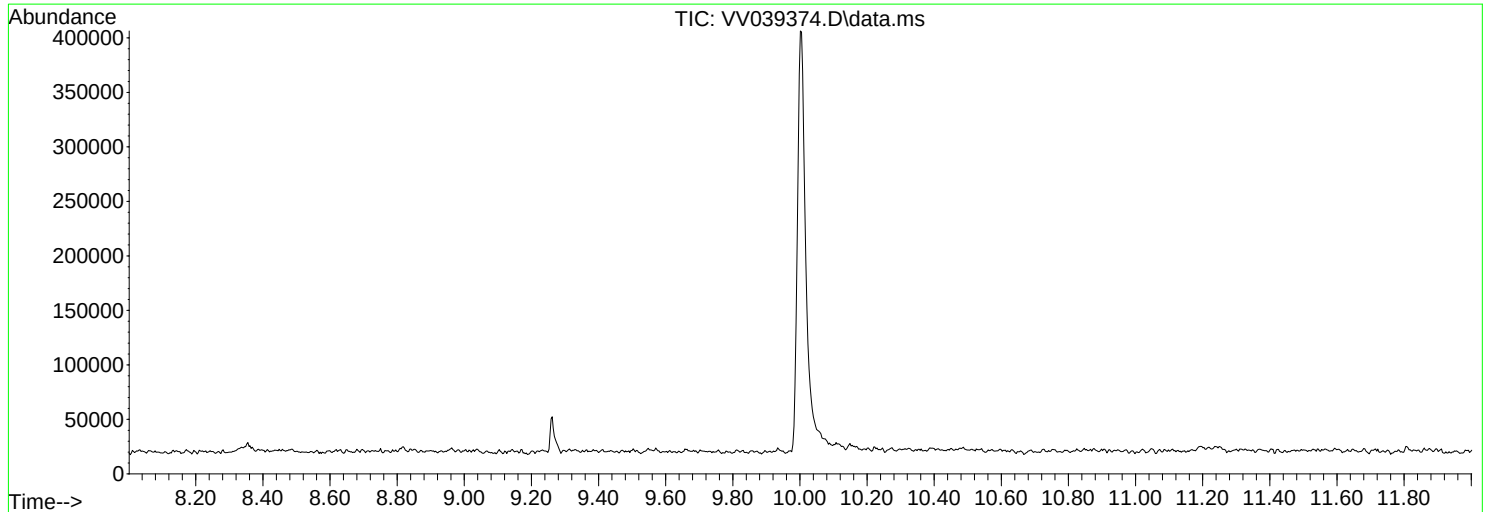

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	12773	PASS
75	95	30	60	46.3	34405	PASS
95	95	100	100	100.0	74264	PASS
96	95	5	9	6.4	4748	PASS
173	174	0.00	2	1.9	1274	PASS
174	95	50	100	89.3	66347	PASS
175	174	5	9	7.7	5093	PASS
176	174	95	101	97.1	64411	PASS
177	176	5	9	7.0	4528	PASS