




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028954.D
 Acq On : 14 Nov 2022 22:05
 Operator : SY/MD
 Sample : N5604-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B0

Manual IntegrationsAPPROVED

Quant Time: Nov 15 05:34:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/15/2022
 Supervised By :Mahesh Dadoda 11/15/2022

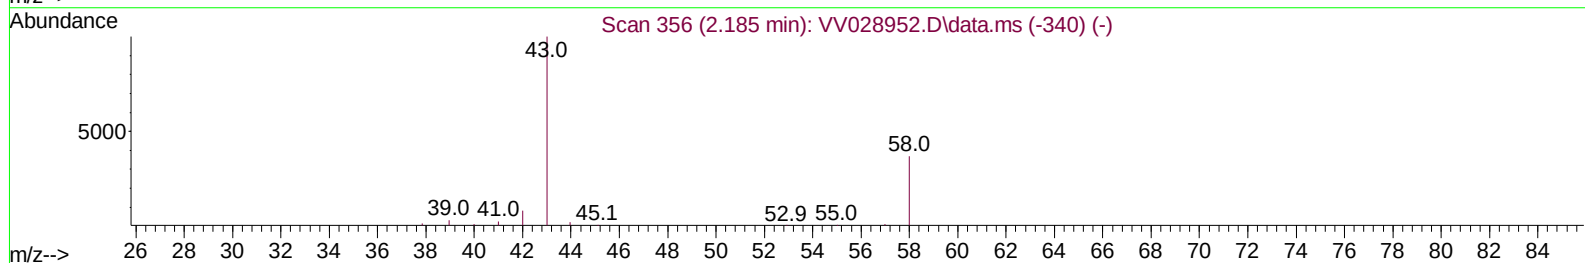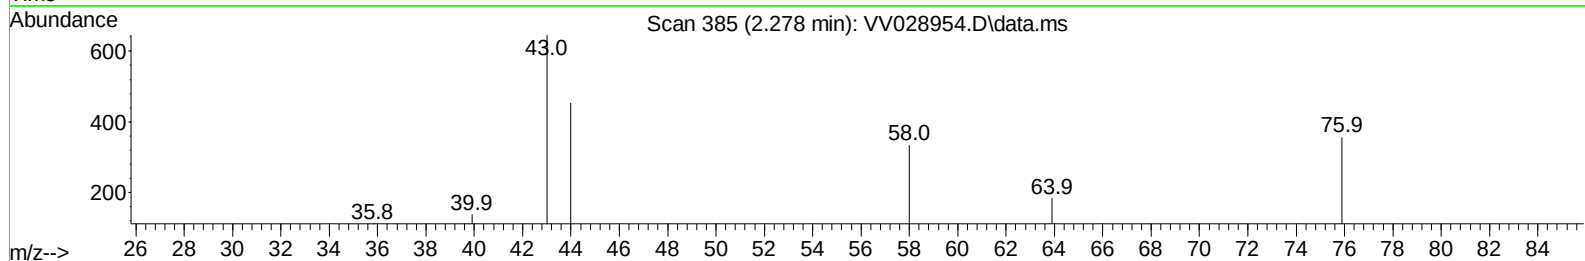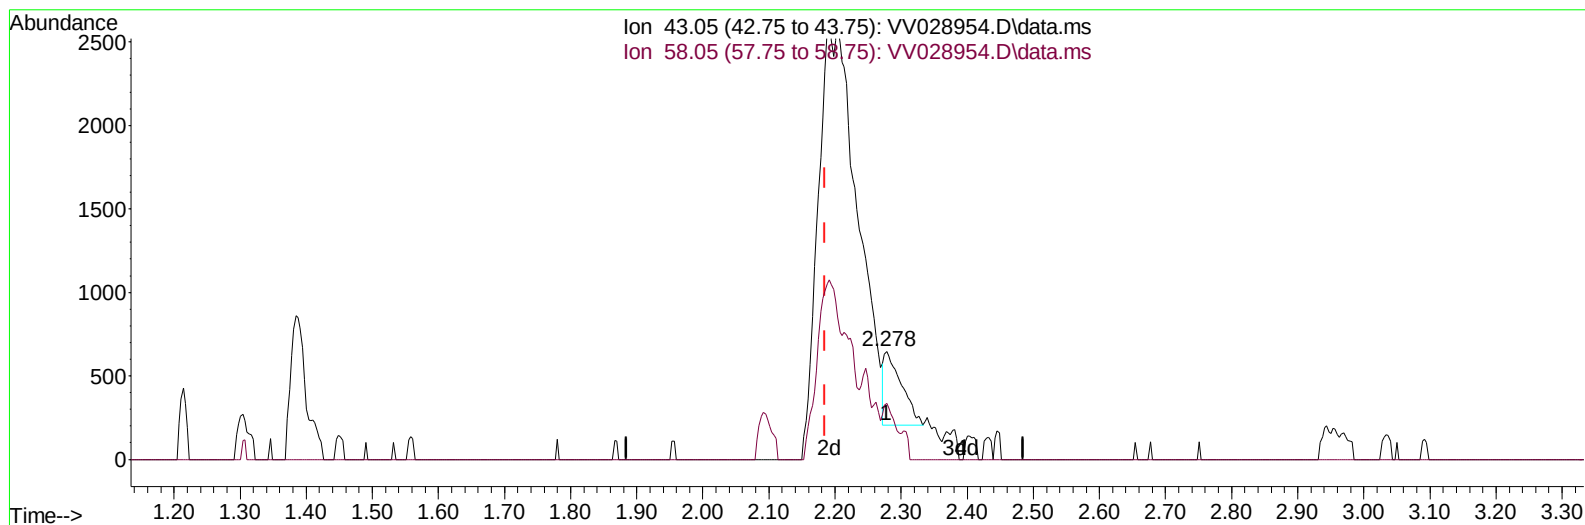

TIC: VV028954.D\data.ms

(13) Acetone (T)

2.278min (+ 0.093) 0.44 ug/L

response 806

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	28.30	24.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028954.D
 Acq On : 14 Nov 2022 22:05
 Operator : SY/MD
 Sample : N5604-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B0

Manual IntegrationsAPPROVED

Quant Time: Nov 15 05:34:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/15/2022
 Supervised By :Mahesh Dadoda 11/15/2022

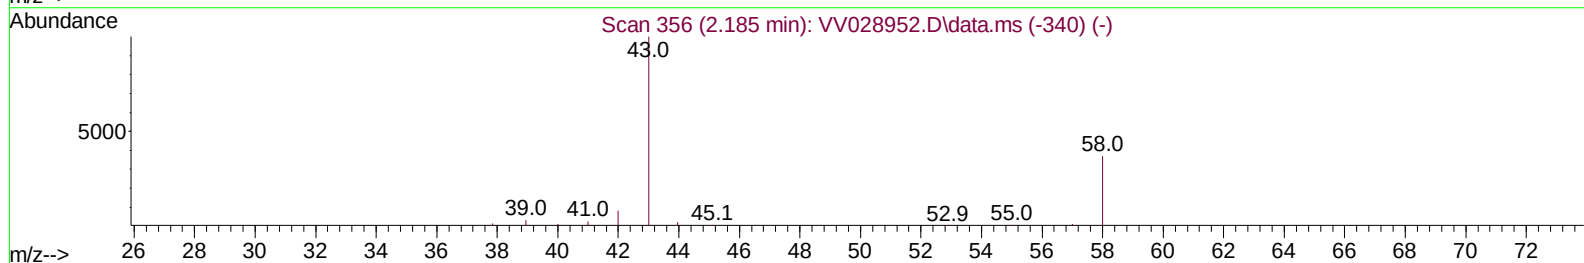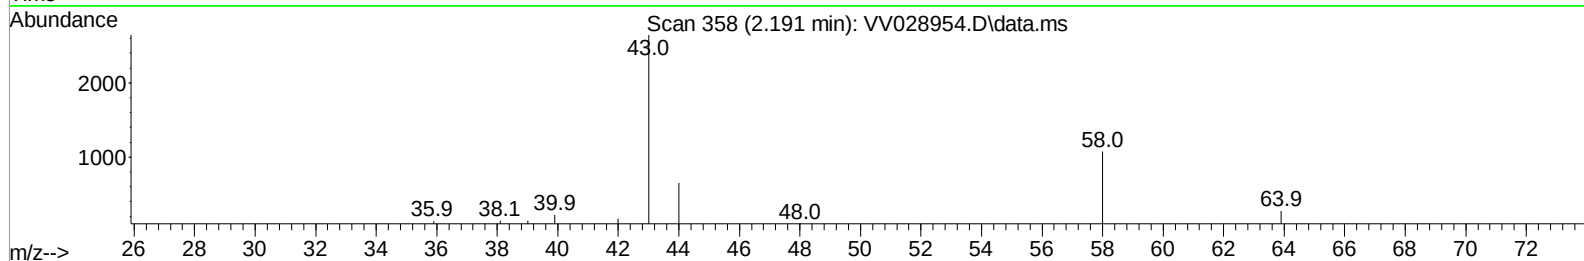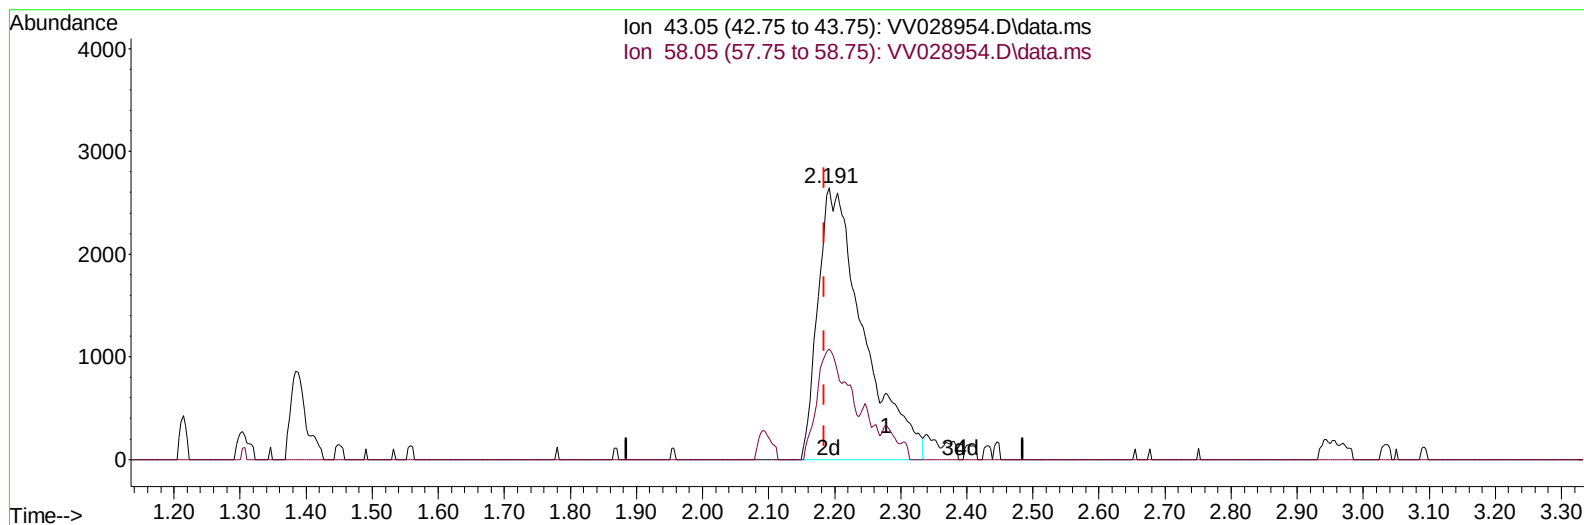

TIC: VV028954.D\data.ms

(13) Acetone (T)

2.191min (+ 0.006) 6.96 ug/L m

response 12628

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	28.30	1.55
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028954.D
 Acq On : 14 Nov 2022 22:05
 Operator : SY/MD
 Sample : N5604-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B0

Manual IntegrationsAPPROVED

Quant Time: Nov 15 05:34:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/15/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		276322	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117		255180	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152		119774	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		59198	3.514	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	70.200%	
7) Chloroethane-d5	1.568	69		62323	4.208	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	84.200%	
11) 1,1-Dichloroethene-d2	2.105	63		87018	2.835	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	56.600%#	
20) 2-Butanone-d5	3.895	46		146034	51.786	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	103.580%	
24) Chloroform-d	4.339	84		160091	4.629	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.027	65		73898	4.749	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	95.000%	
32) Benzene-d6	5.043	84		325418	4.272	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	6.063	67		95801	4.504	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	90.000%	
41) Toluene-d8	7.310	98		285957	4.171	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	83.400%	
43) trans-1,3-Dichloroprop...	7.619	79		29004	4.181	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	83.600%	
46) 2-Hexanone-d5	8.085	63		135725	45.838	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	91.680%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84		69824	4.735	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.615	152		103357	4.823	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	96.400%	
Target Compounds							
13) Acetone	2.191	43		12628m	6.961	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028954.D
Acq On : 14 Nov 2022 22:05
Operator : SY/MD
Sample : N5604-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46B0

Manual IntegrationsAPPROVED

Quant Time: Nov 15 05:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 15 01:23:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/15/2022
Supervised By :Mahesh Dadoda 11/15/2022

