

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111422\
 Data File : VW028932.D
 Acq On : 14 Nov 2022 12:42
 Operator : SY/MD
 Sample : N5590-10DL 25X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBMY1DL

Quant Time: Nov 15 00:03:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 00:01:45 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	269082	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	243634	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	122734	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61172	3.729	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	74.600%	
7) Chloroethane-d5	1.568	69	62186	4.312	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.200%	
11) 1,1-Dichloroethene-d2	2.104	63	90514	3.028	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.600%	
20) 2-Butanone-d5	3.895	46	149329	54.380	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.760%	
24) Chloroform-d	4.342	84	156131	4.636	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.800%	
26) 1,2-Dichloroethane-d4	5.030	65	72487	4.784	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
32) Benzene-d6	5.046	84	329856	4.536	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.800%	
36) 1,2-Dichloropropane-d6	6.066	67	94673	4.662	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.200%	
41) Toluene-d8	7.310	98	291335	4.450	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	7.622	79	29998	4.529	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.088	63	127499	45.100	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.200%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	67787	4.815	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.200%	
66) 1,2-Dichlorobenzene-d4	11.615	152	106957	4.871	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.400%	
Target Compounds						
					Qvalue	
13) Acetone	2.191	43	7303	4.134	ug/L	76
16) Methylene chloride	2.506	84	28033	1.331	ug/L	94
22) cis-1,2-Dichloroethene	3.918	96	8681	0.452	ug/L	97
30) Cyclohexane	4.670	56	24549	0.845	ug/L	94
33) Benzene	5.095	78	1159089	15.569	ug/L	100
35) Methylcyclohexane	6.127	83	3953	0.118	ug/L #	62
60) Isopropylbenzene	9.931	105	6852	0.086	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028932.D
Acq On : 14 Nov 2022 12:42
Operator : SY/MD
Sample : N5590-10DL 25X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY1DL

Quant Time: Nov 15 00:03:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 15 00:01:45 2022
Response via : Initial Calibration

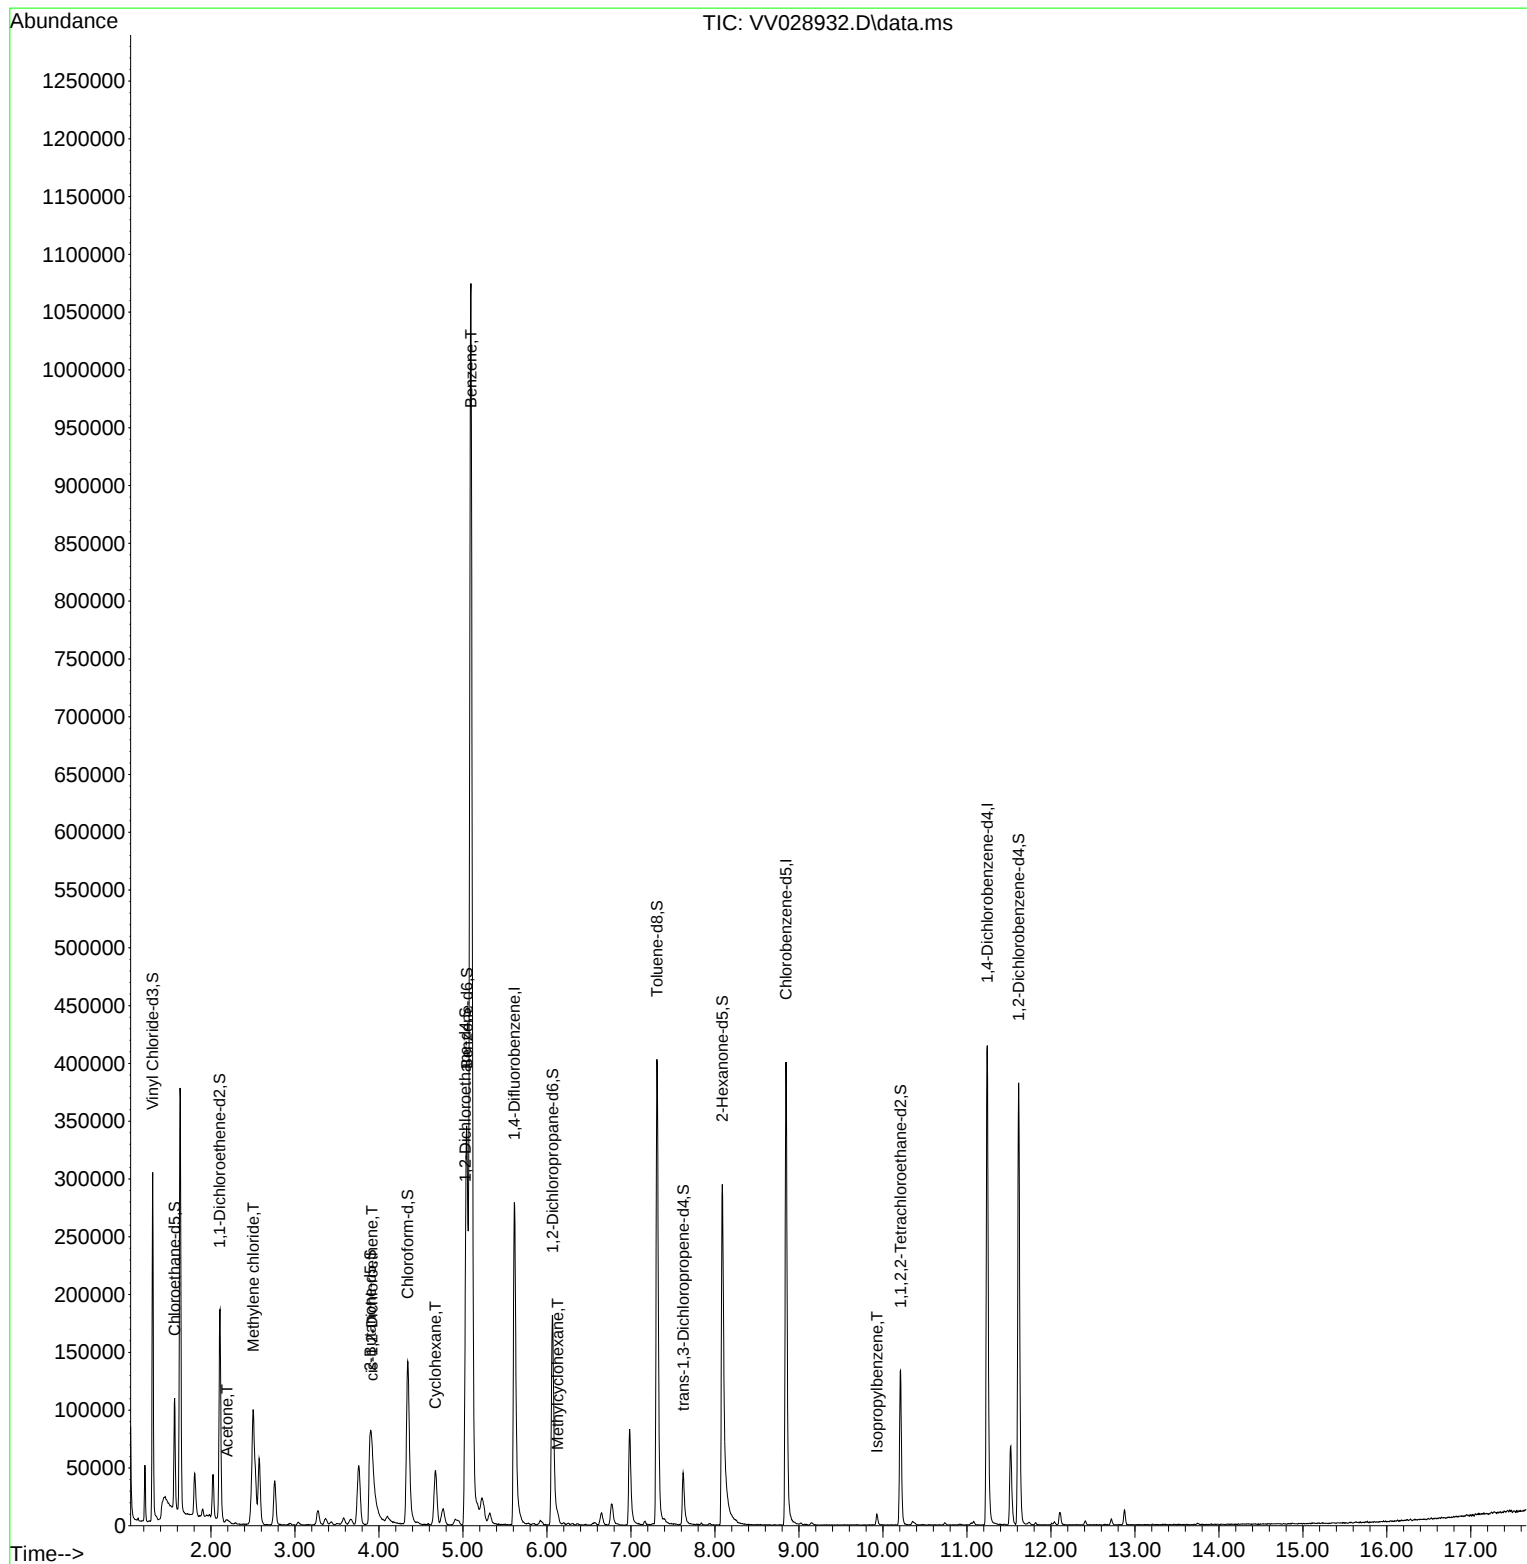

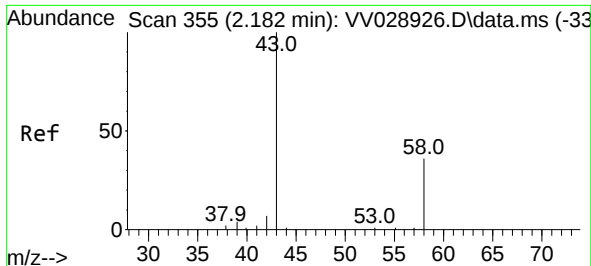

#13

Acetone

Concen: 4.134 ug/L

RT: 2.191 min Scan# 3

Delta R.T. 0.009 min

Lab File: VV028932.D

Acq: 14 Nov 2022 12:42

Instrument :

MSVOA_V

ClientSampleId :





GBMY1DL

Tgt Ion: 43 Resp: 7303

Ion Ratio Lower Upper

43 100

58 15.4 0.0 56.6

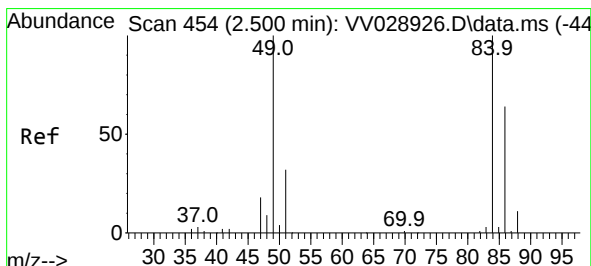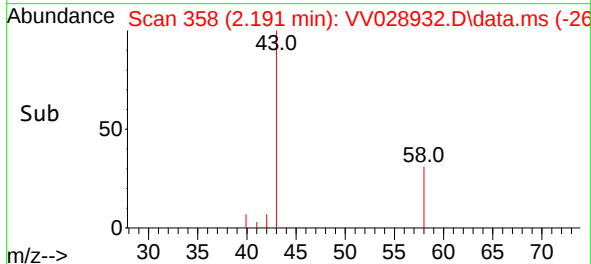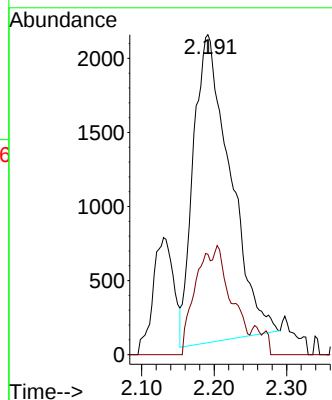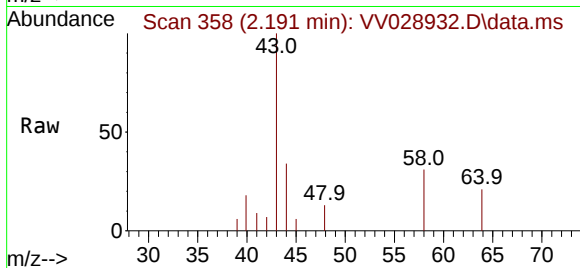

#16

Methylene chloride

Concen: 1.331 ug/L

RT: 2.506 min Scan# 456

Delta R.T. 0.006 min

Lab File: VV028932.D

Acq: 14 Nov 2022 12:42




Tgt Ion: 84 Resp: 28033


Ion Ratio Lower Upper

84 100

86 69.9 45.8 85.0

49 101.0 75.5 140.1

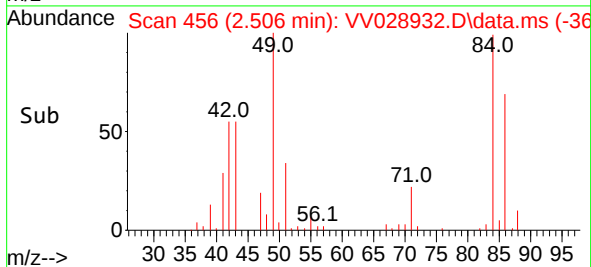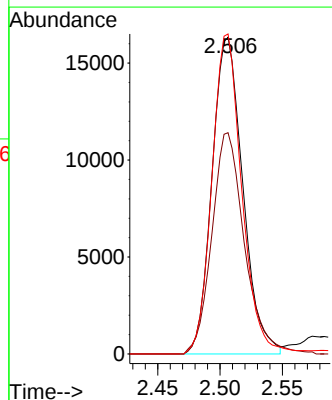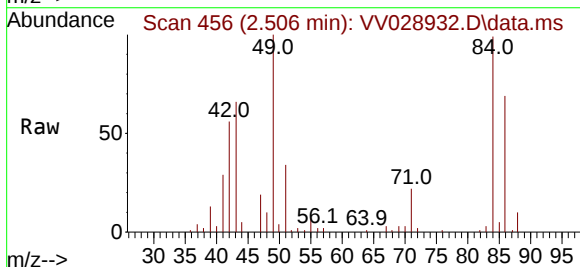

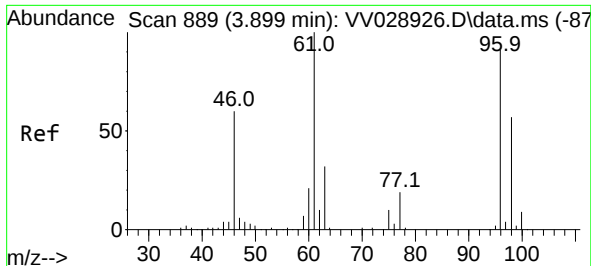

#22

cis-1,2-Dichloroethene

Concen: 0.452 ug/L

RT: 3.918 min Scan# 895

Delta R.T. 0.019 min

Lab File: VV028932.D

Acq: 14 Nov 2022 12:42

Instrument :

MSVOA_V

ClientSampleId :

GBMY1DL





Tgt Ion: 96 Resp: 8681

Ion Ratio Lower Upper

96 100

61 114.6 82.3 152.9

68 0.0 0.0 0.0

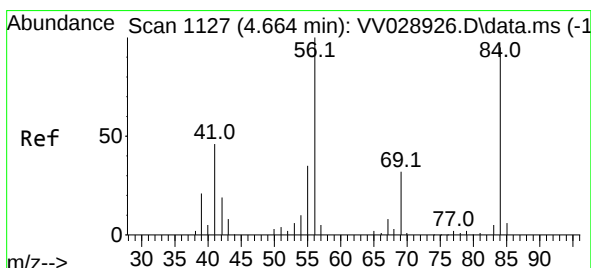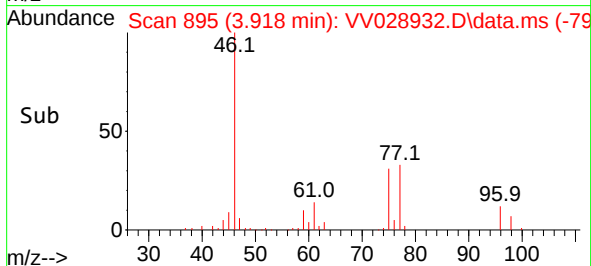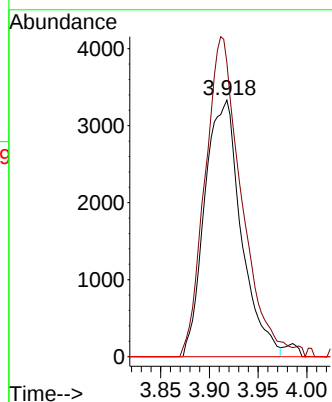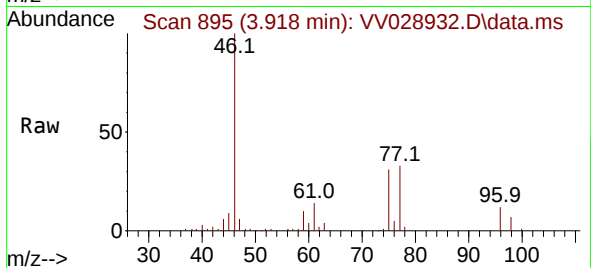

#30

Cyclohexane

Concen: 0.845 ug/L

RT: 4.670 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VV028932.D

Acq: 14 Nov 2022 12:42




Tgt Ion: 56 Resp: 24549


Ion Ratio Lower Upper

56 100

69 34.5 26.1 39.1

84 103.7 77.9 116.9


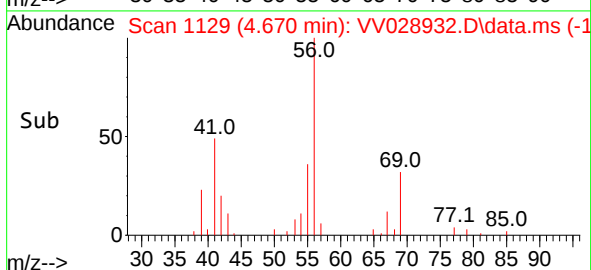
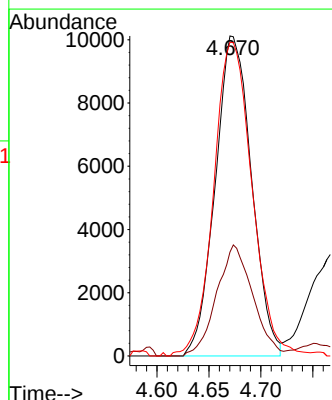
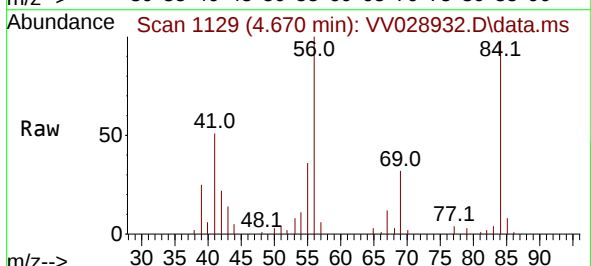


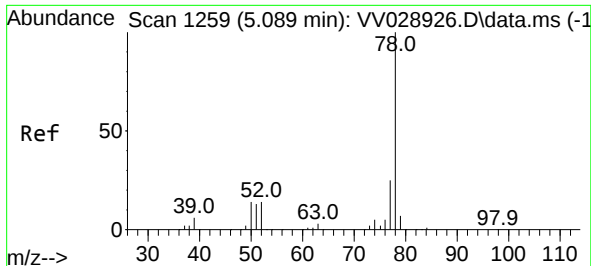

#33
Benzene
Concen: 15.569 ug/L
RT: 5.095 min Scan# 11
Delta R.T. 0.006 min
Lab File: VV028932.D
Acq: 14 Nov 2022 12:42




Instrument :
MSVOA_V
ClientSampleId :
GBMY1DL


Tgt Ion: 78 Resp: 1159089

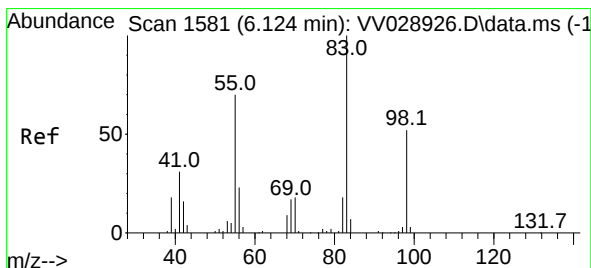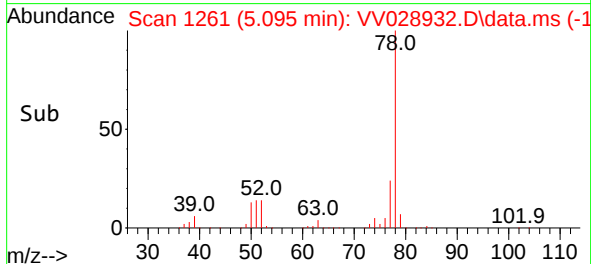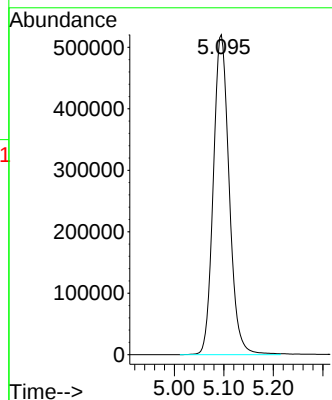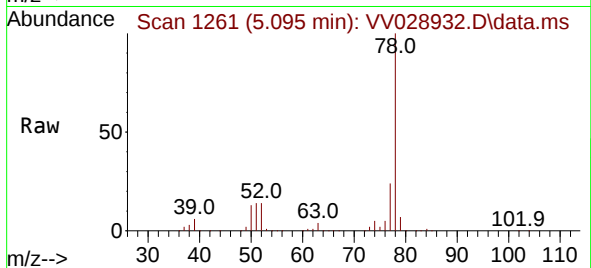

#35
Methylcyclohexane
Concen: 0.118 ug/L
RT: 6.127 min Scan# 1582
Delta R.T. 0.003 min
Lab File: VV028932.D
Acq: 14 Nov 2022 12:42

Tgt Ion: 83 Resp: 3953
Ion Ratio Lower Upper
83 100
55 100.6 55.8 83.6#
98 22.2 38.2 57.2#

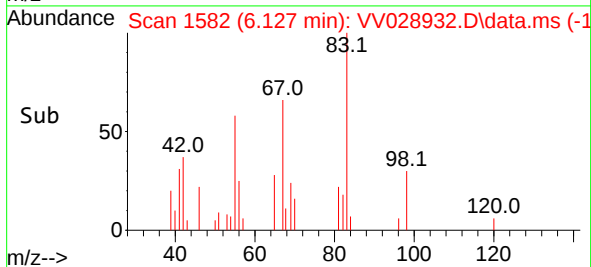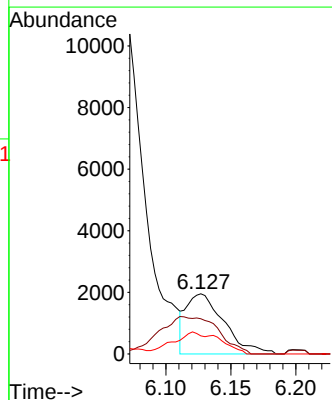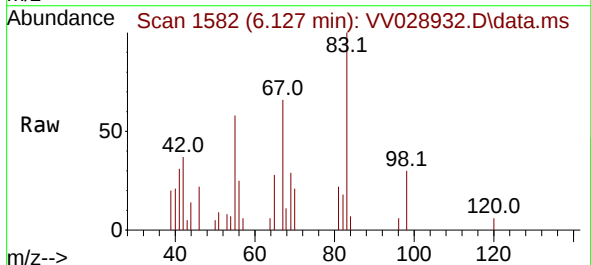

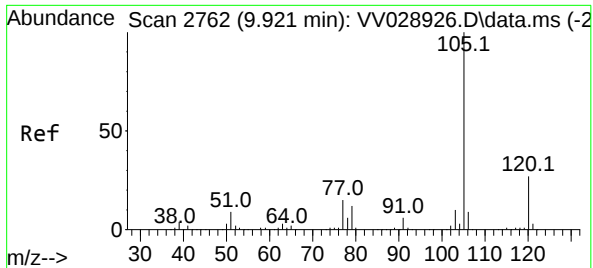

#60
 Isopropylbenzene
 Concen: 0.086 ug/L
 RT: 9.931 min Scan# 21
 Delta R.T. 0.009 min
 Lab File: VV028932.D
 Acq: 14 Nov 2022 12:42

Instrument :
 MSVOA_V
 ClientSampleId :
 GBMY1DL

Tgt Ion:	105	Resp:	6852
Ion	Ratio	Lower	Upper
105	100		
120	25.1	21.3	31.9
77	15.7	11.8	17.8

