

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028953.D
 Acq On : 14 Nov 2022 21:37
 Operator : SY/MD
 Sample : VV1114WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK262

Quant Time: Nov 15 01:23:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	279413	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	260260	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	126182	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73047	4.288	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.800%	
7) Chloroethane-d5	1.568	69	71917	4.802	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.000%	
11) 1,1-Dichloroethene-d2	2.105	63	104702	3.373	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.400%	
20) 2-Butanone-d5	3.899	46	102363	35.898	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	71.800%	
24) Chloroform-d	4.343	84	171930	4.916	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	5.027	65	80564	5.120	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.400%	
32) Benzene-d6	5.047	84	373915	4.813	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
36) 1,2-Dichloropropane-d6	6.066	67	107395	4.951	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.000%	
41) Toluene-d8	7.310	98	334041	4.777	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
43) trans-1,3-Dichloroprop...	7.622	79	33495	4.734	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.088	63	149018	49.345	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.700%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	75655	5.030	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.600%	
66) 1,2-Dichlorobenzene-d4	11.616	152	120570	5.341	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.800%	
Target Compounds						
16) Methylene chloride	2.507	84	4157	0.190	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028953.D
Acq On : 14 Nov 2022 21:37
Operator : SY/MD
Sample : VV1114WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK262


Quant Time: Nov 15 01:23:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 15 01:23:16 2022
Response via : Initial Calibration

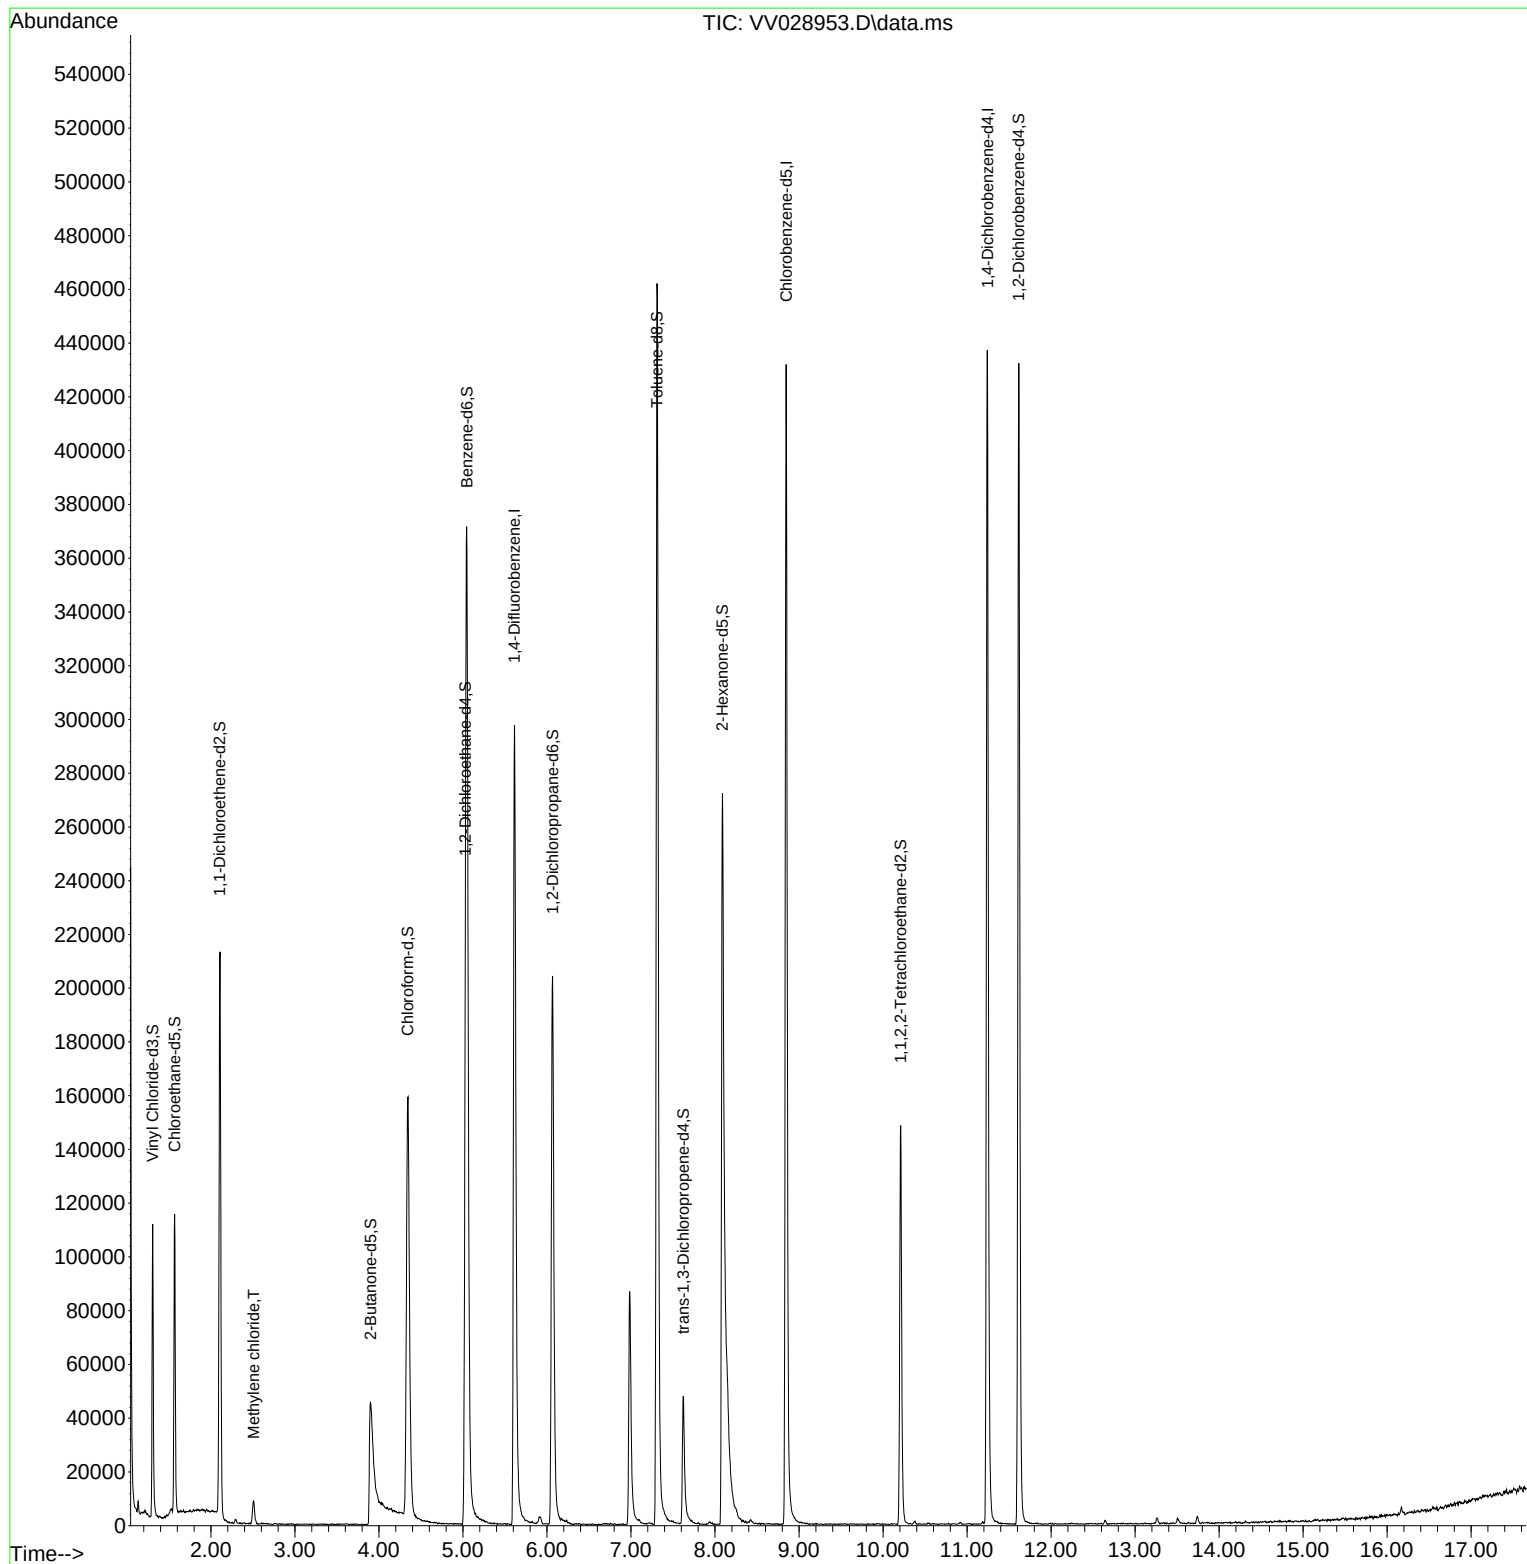

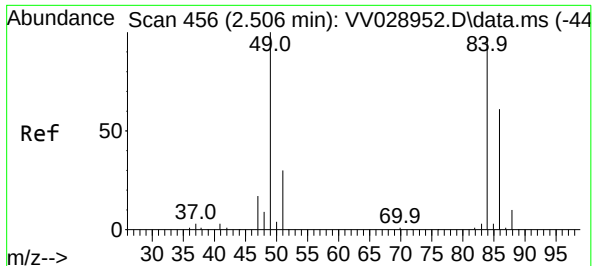

#16
Methylene chloride
Concen: 0.190 ug/L
RT: 2.507 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028953.D
Acq: 14 Nov 2022 21:37

Instrument :
MSVOA_V
ClientSampleId :
VBLK262

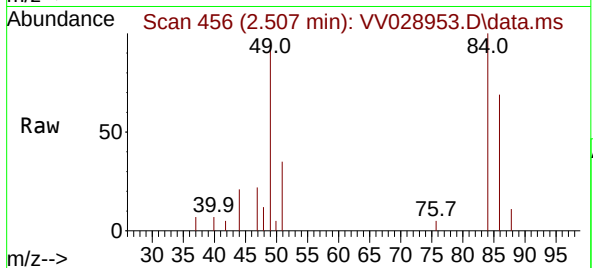

Tgt Ion:	84	Resp:	4157
Ion	Ratio	Lower	Upper
84	100		
86	69.4	45.8	85.0
49	96.1	75.5	140.1

