

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111422\
 Data File : VW028954.D
 Acq On : 14 Nov 2022 22:05
 Operator : SY/MD
 Sample : N5604-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B0

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 11/15/2022
 Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 15 05:34:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	276322	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	255180	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	119774	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	59198	3.514	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	70.200%	
7) Chloroethane-d5	1.568	69	62323	4.208	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.200%	
11) 1,1-Dichloroethene-d2	2.105	63	87018	2.835	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.600%#	
20) 2-Butanone-d5	3.895	46	146034	51.786	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.580%	
24) Chloroform-d	4.339	84	160091	4.629	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.600%	
26) 1,2-Dichloroethane-d4	5.027	65	73898	4.749	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.000%	
32) Benzene-d6	5.043	84	325418	4.272	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	6.063	67	95801	4.504	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.000%	
41) Toluene-d8	7.310	98	285957	4.171	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.400%	
43) trans-1,3-Dichloroprop...	7.619	79	29004	4.181	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.085	63	135725	45.838	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.680%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	69824	4.735	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.615	152	103357	4.823	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.400%	
Target Compounds					Qvalue	
13) Acetone	2.191	43	12628m	6.961	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028954.D
Acq On : 14 Nov 2022 22:05
Operator : SY/MD
Sample : N5604-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
H46B0

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 11/15/2022
Supervised By :Mahesh Dadoda 11/15/2022

Quant Time: Nov 15 05:34:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 15 01:23:16 2022
Response via : Initial Calibration

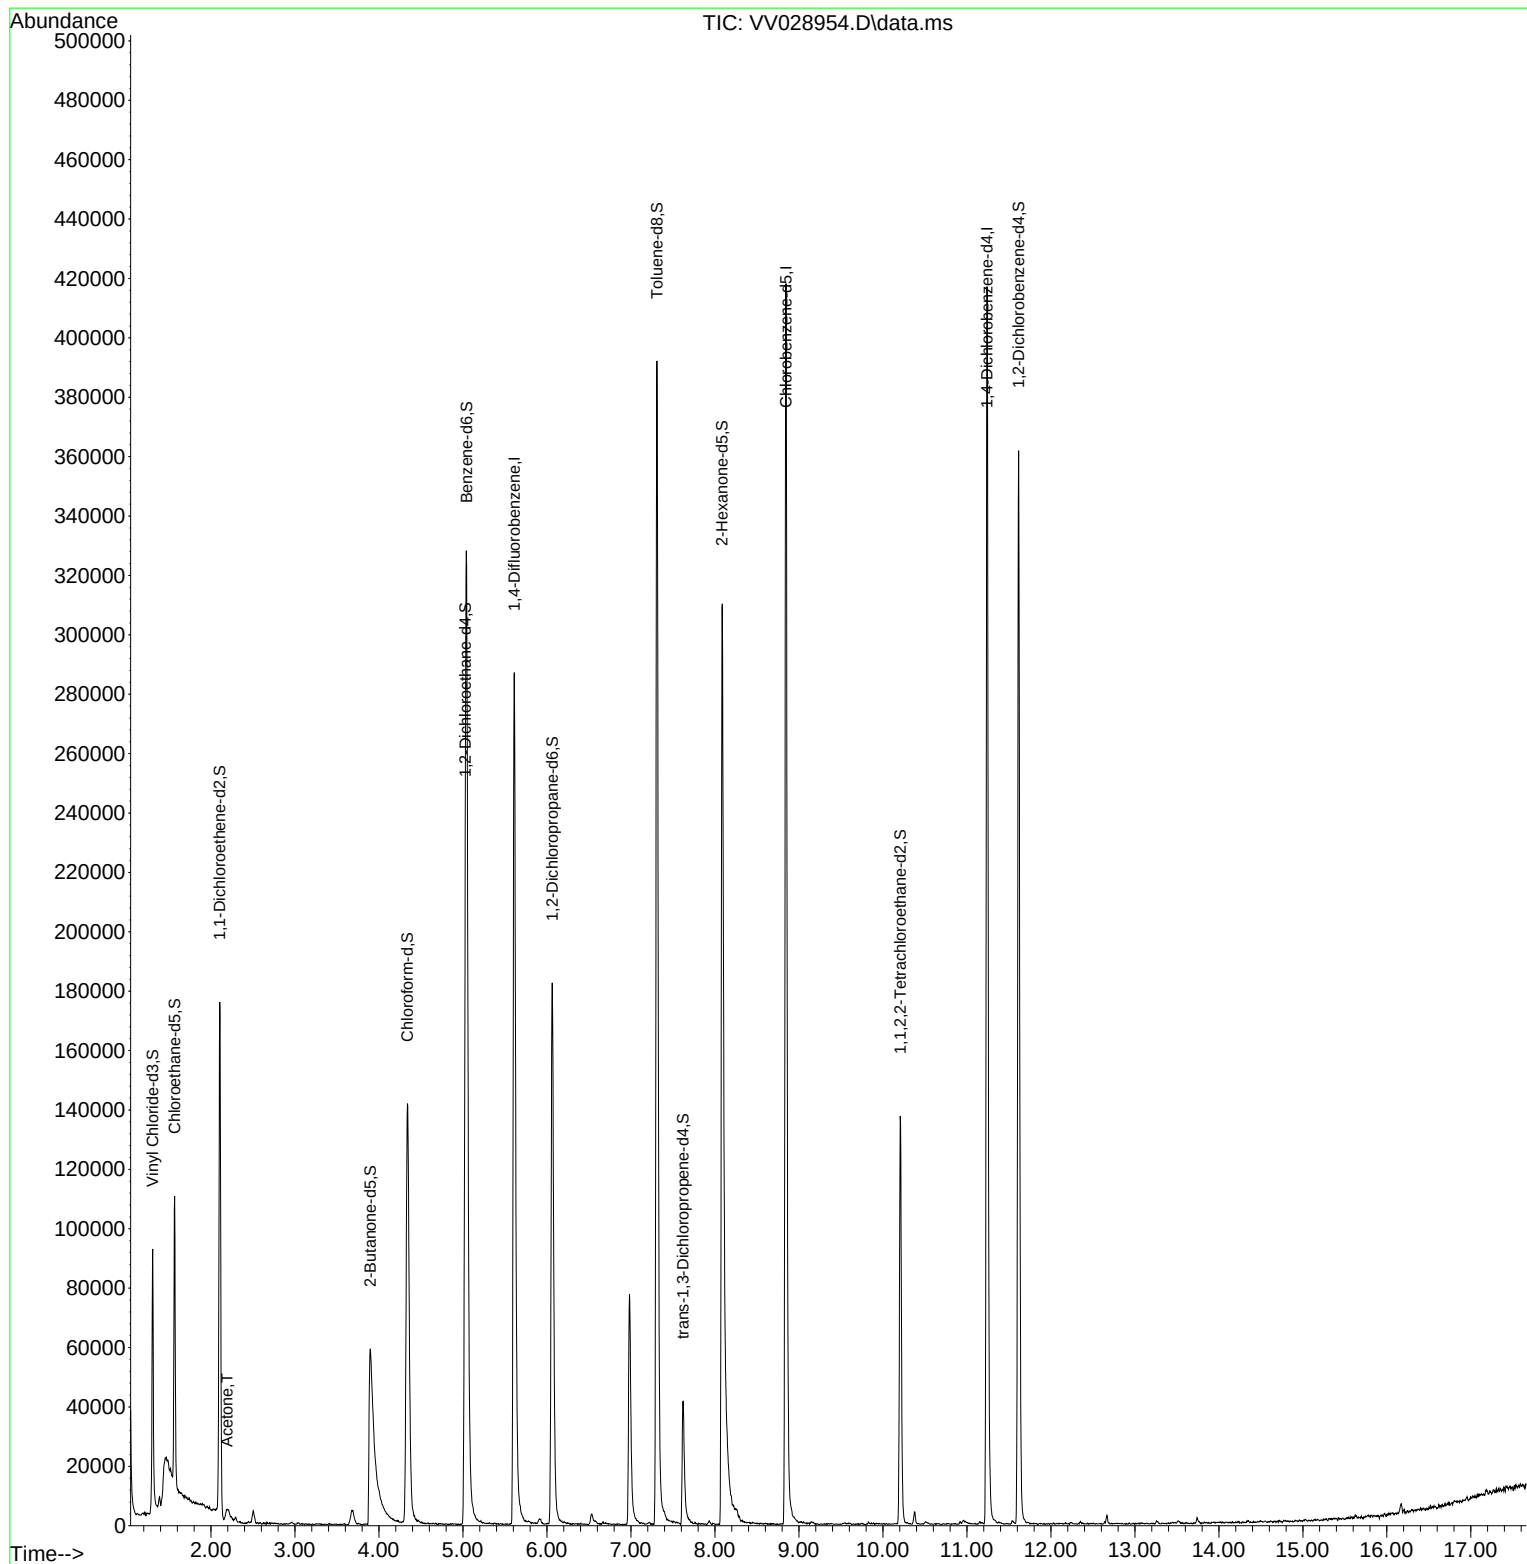

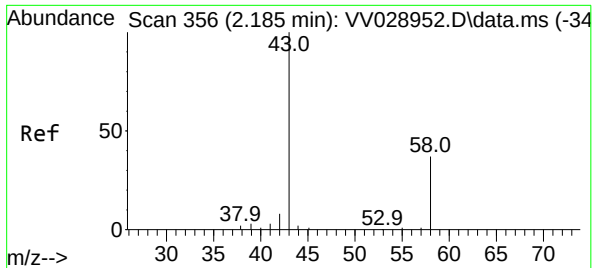

#13
 Acetone
 Concen: 6.961 ug/L m
 RT: 2.191 min Scan# 3
 Delta R.T. 0.006 min
 Lab File: VV028954.D
 Acq: 14 Nov 2022 22:05

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B0

Tgt Ion: 43 Resp: 12628
 Ion Ratio Lower Upper
 43 100
 58 1.6 0.0 56.6

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 11/15/2022
 Supervised By :Mahesh Dadoda 11/15/2022

