

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111422\
 Data File : VW028966.D
 Acq On : 15 Nov 2022 02:59
 Operator : SY/MD
 Sample : N5604-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B1

Quant Time: Nov 15 05:37:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 15 01:23:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	272593	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	248393	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	114643	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	58951	3.547	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.000%
7) Chloroethane-d5	1.568	69	61632	4.219	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.400%
11) 1,1-Dichloroethene-d2	2.105	63	87039	2.874	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.400%#
20) 2-Butanone-d5	3.896	46	159647	57.388	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.780%
24) Chloroform-d	4.343	84	159652	4.679	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
26) 1,2-Dichloroethane-d4	5.027	65	73686	4.800	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	5.047	84	323797	4.367	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.400%
36) 1,2-Dichloropropane-d6	6.066	67	96663	4.669	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.400%
41) Toluene-d8	7.310	98	281506	4.218	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.400%
43) trans-1,3-Dichloroprop...	7.622	79	26516	3.927	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.600%
46) 2-Hexanone-d5	8.088	63	130342	45.223	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.440%
56) 1,1,2,2-Tetrachloroeth...	10.211	84	65049	4.532	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.600%
66) 1,2-Dichlorobenzene-d4	11.616	152	100978	4.923	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.400%
Target Compounds						
					Qvalue	
13) Acetone	2.192	43	11230	6.276	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028966.D
Acq On : 15 Nov 2022 02:59
Operator : SY/MD
Sample : N5604-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46B1

Quant Time: Nov 15 05:37:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 15 01:23:16 2022
Response via : Initial Calibration

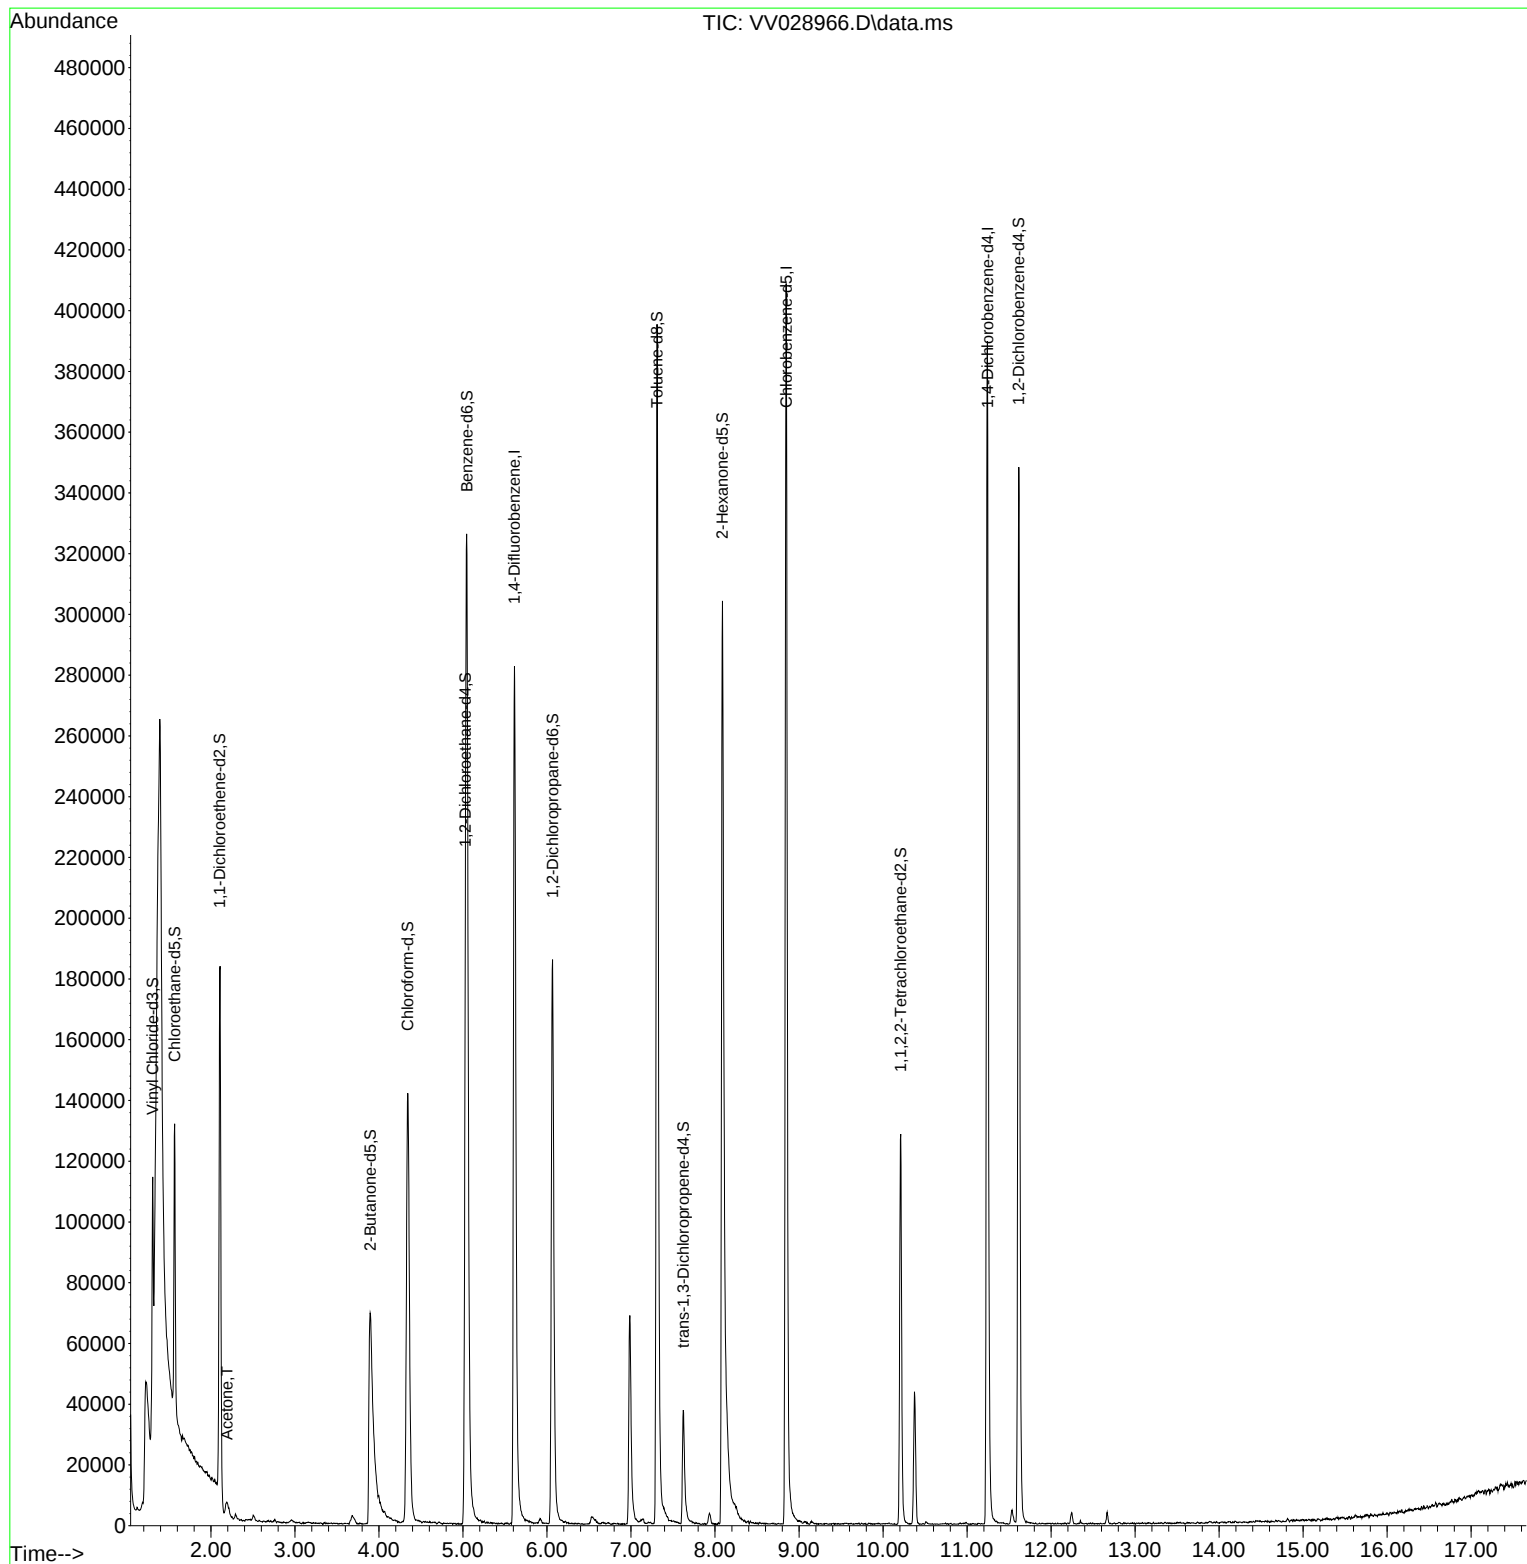

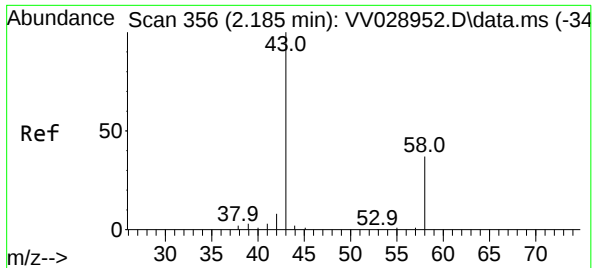

#13
 Acetone
 Concen: 6.276 ug/L
 RT: 2.192 min Scan# 311
 Delta R.T. 0.007 min
 Lab File: VV028966.D
 Acq: 15 Nov 2022 02:59

Instrument :
 MSVOA_V
 ClientSampleId :
 H46B1

Tgt Ion: 43 Resp: 11230
 Ion Ratio Lower Upper
 43 100
 58 33.8 0.0 56.6

