

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028927.D
 Acq On : 14 Nov 2022 10:32
 Operator : SY/MD
 Sample : VV1114WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	100755	107550	13.06%	1.653%
2	1.429	108	121	126	rBV2	14140	35955	4.37%	0.553%
3	1.565	156	163	178	rVB	102038	118224	14.36%	1.817%
4	2.105	321	331	347	rVB	200357	298160	36.21%	4.583%
5	2.503	445	455	465	rBV2	7285	12182	1.48%	0.187%
6	3.892	873	887	919	rBV	33988	131664	15.99%	2.024%
7	4.339	1008	1026	1052	rVB2	139845	349029	42.39%	5.365%
8	5.040	1227	1244	1277	rBV2	325052	823421	100.00%	12.657%
9	5.609	1408	1421	1457	rBV	276015	571453	69.40%	8.784%
10	6.063	1549	1562	1594	rBV	179191	375377	45.59%	5.770%
11	6.982	1837	1848	1874	rBV	80121	154308	18.74%	2.372%
12	7.310	1937	1950	1970	rBV	397423	711411	86.40%	10.935%
13	7.619	2037	2046	2071	rBV2	43757	83662	10.16%	1.286%
14	8.088	2182	2192	2239	rBV	211277	623541	75.73%	9.584%
15	8.844	2416	2427	2459	rBV	390726	673003	81.73%	10.345%
16	10.210	2840	2852	2876	rBV	118406	197933	24.04%	3.042%
17	11.243	3162	3173	3195	rVV	391021	640731	77.81%	9.848%
18	11.616	3278	3289	3311	rBV	360034	578207	70.22%	8.887%
19	13.503	3865	3876	3885	rBV2	5632	9812	1.19%	0.151%
20	13.738	3938	3949	3962	rBV5	6285	10271	1.25%	0.158%




Sum of corrected areas: 6505894

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028927.D
Acq On : 14 Nov 2022 10:32
Operator : SY/MD
Sample : VV1114WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

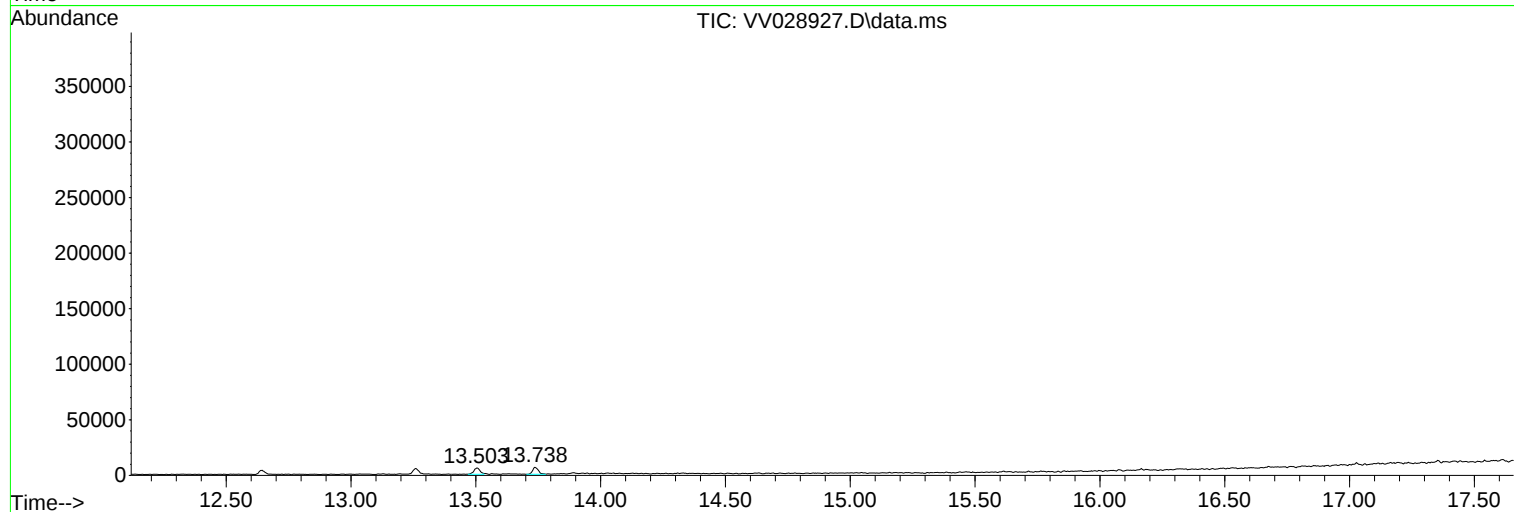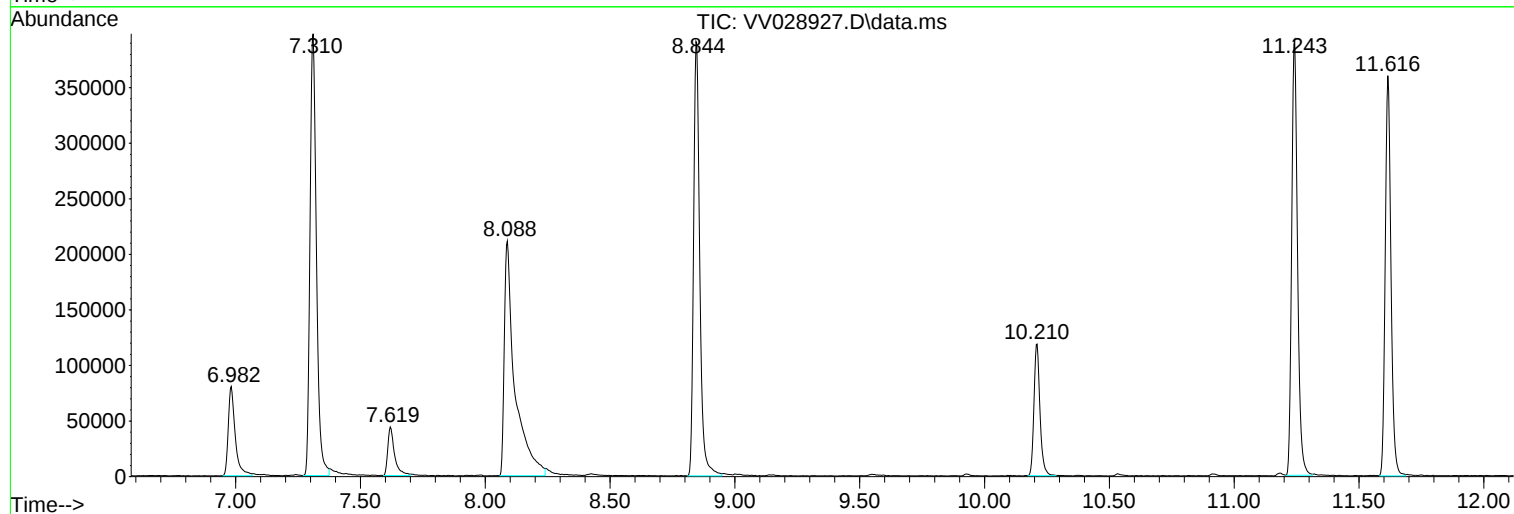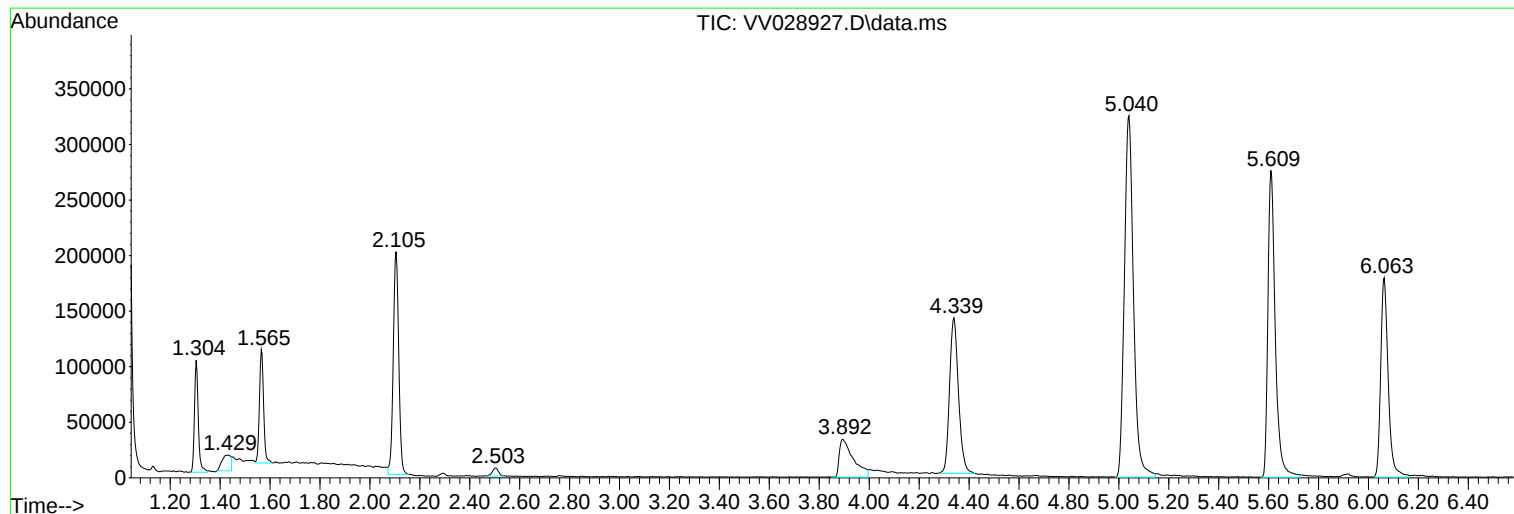

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028927.D
Acq On : 14 Nov 2022 10:32
Operator : SY/MD
Sample : VV1114WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028927.D
Acq On : 14 Nov 2022 10:32
Operator : SY/MD
Sample : VV1114WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc