

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028934.D
 Acq On : 14 Nov 2022 13:31
 Operator : SY/MD
 Sample : N5590-12DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBMY3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	96	rBV	82598	88569	11.35%	1.216%
2	1.465	112	132	134	rBV	8369	24363	3.12%	0.335%
3	1.564	155	163	178	rVB	86636	103834	13.31%	1.426%
4	1.986	287	294	306	rVB2	13203	19353	2.48%	0.266%
5	2.101	320	330	347	rVB	175489	257151	32.97%	3.532%
6	2.500	442	454	478	rVB	45867	79333	10.17%	1.090%
7	3.905	874	891	925	rBV5	180050	549680	70.47%	7.549%
8	4.339	1010	1026	1057	rVB	128926	333254	42.72%	4.577%
9	5.040	1229	1244	1269	rBV2	310138	780053	100.00%	10.714%
10	5.613	1407	1422	1450	rBV	269154	551587	70.71%	7.576%
11	5.908	1501	1514	1542	rBV	247131	502256	64.39%	6.898%
12	6.066	1550	1563	1586	rBV	169335	349519	44.81%	4.800%
13	6.985	1839	1849	1876	rBV	75991	148539	19.04%	2.040%
14	7.310	1939	1950	1979	rBV	380768	683141	87.58%	9.382%
15	7.622	2037	2047	2066	rBV2	41566	78172	10.02%	1.074%
16	8.088	2179	2192	2235	rBV	270431	643188	82.45%	8.834%
17	8.420	2284	2295	2310	rBV2	7537	14913	1.91%	0.205%
18	8.847	2416	2428	2461	rBV	388112	651356	83.50%	8.946%
19	10.210	2840	2852	2875	rBV2	125233	204002	26.15%	2.802%
20	11.243	3161	3173	3197	rBV	402275	642203	82.33%	8.820%
21	11.616	3276	3289	3317	rBV	353021	576549	73.91%	7.919%




Sum of corrected areas: 7281015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028934.D
Acq On : 14 Nov 2022 13:31
Operator : SY/MD
Sample : N5590-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

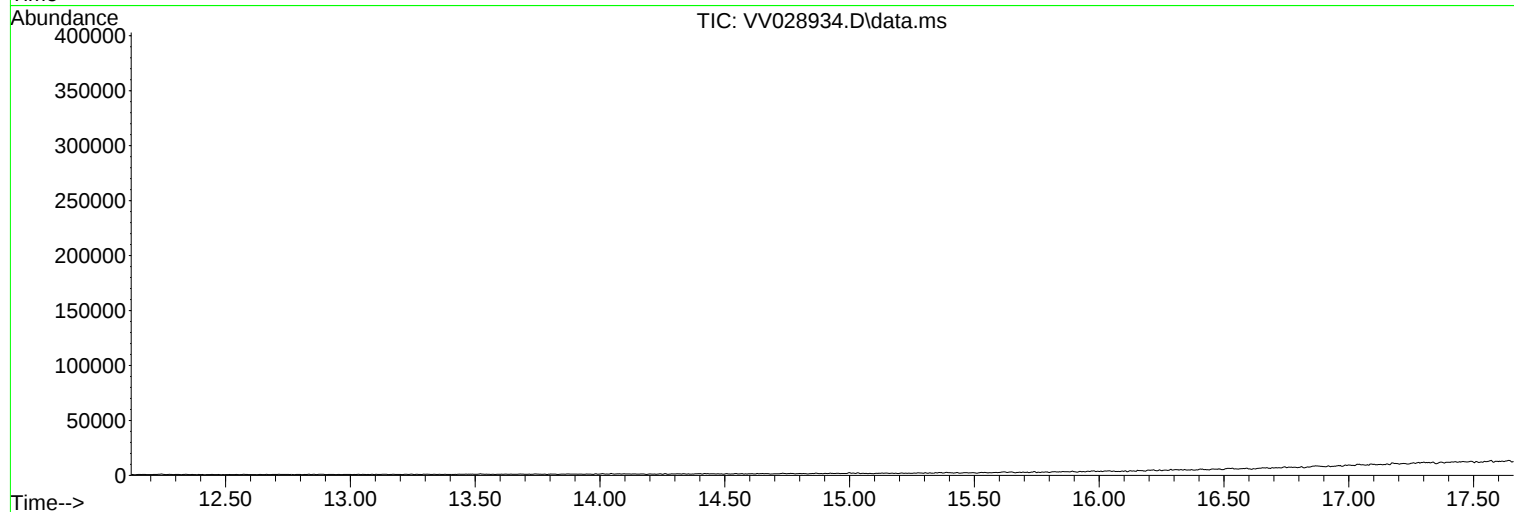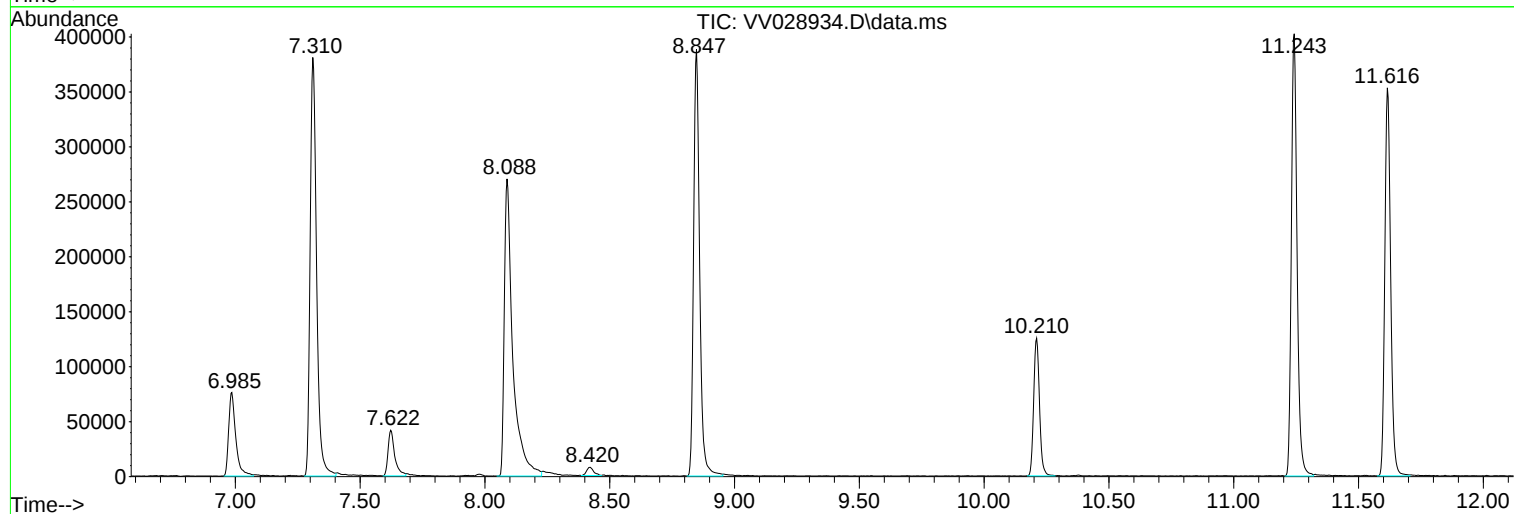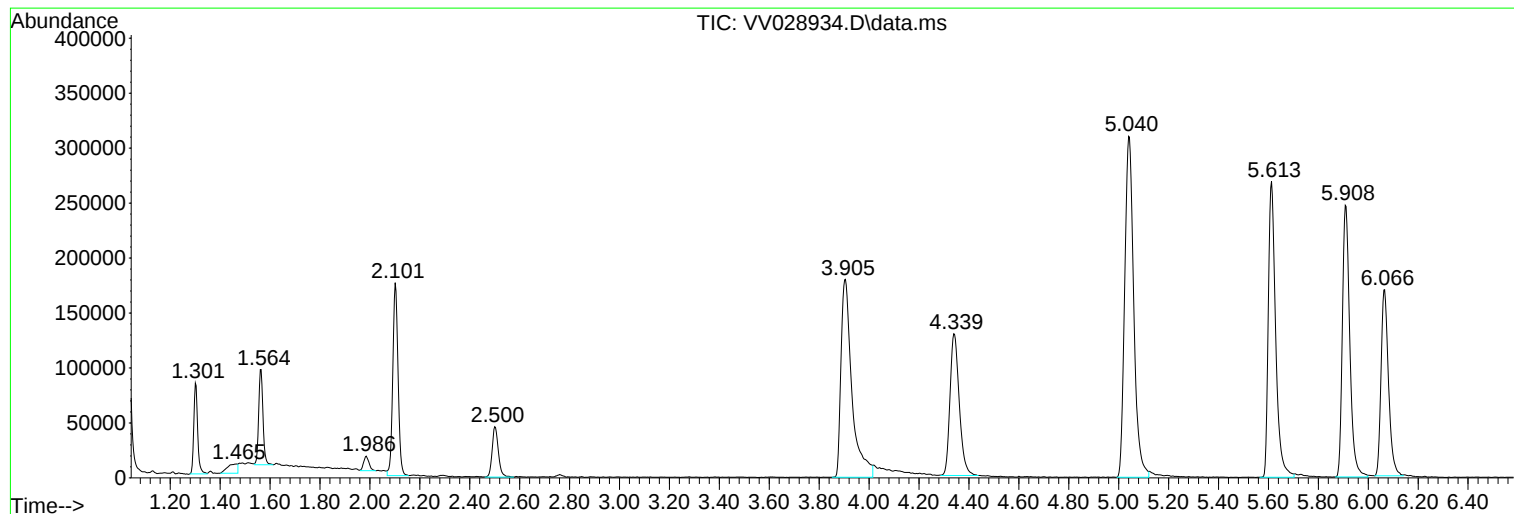

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028934.D
Acq On : 14 Nov 2022 13:31
Operator : SY/MD
Sample : N5590-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028934.D
Acq On : 14 Nov 2022 13:31
Operator : SY/MD
Sample : N5590-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBMY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc