

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028937.D
 Acq On : 14 Nov 2022 14:45
 Operator : SY/MD
 Sample : N5590-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	94874	102521	11.90%	1.463%
2	1.471	115	134	135	rBV2	12300	29971	3.48%	0.428%
3	1.568	157	164	176	rVB	102674	119940	13.92%	1.712%
4	2.105	321	331	347	rVB	193387	285495	33.13%	4.075%
5	2.507	445	456	467	rBV	19414	31183	3.62%	0.445%
6	3.889	876	886	936	rBV	70781	275699	31.99%	3.936%
7	4.342	1010	1027	1059	rBV	147649	373056	43.29%	5.325%
8	5.043	1229	1245	1276	rBV2	342289	861767	100.00%	12.302%
9	5.612	1408	1422	1455	rBV	283879	591068	68.59%	8.438%
10	6.066	1550	1563	1592	rBV	189065	397653	46.14%	5.677%
11	6.982	1838	1848	1883	rBV	83126	164235	19.06%	2.344%
12	7.310	1938	1950	1979	rBV	420783	752659	87.34%	10.744%
13	7.619	2037	2046	2070	rBV	45558	85990	9.98%	1.228%
14	8.088	2179	2192	2228	rBV	298205	700276	81.26%	9.996%
15	8.847	2414	2428	2458	rBV	407179	689764	80.04%	9.846%
16	10.210	2838	2852	2871	rBV2	136029	222836	25.86%	3.181%
17	11.242	3160	3173	3200	rBV	404658	673194	78.12%	9.610%
18	11.615	3272	3289	3311	rBV	374042	614790	71.34%	8.776%
19	16.168	4697	4705	4718	rVB3	20308	33148	3.85%	0.473%




Sum of corrected areas: 7005245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028937.D
Acq On : 14 Nov 2022 14:45
Operator : SY/MD
Sample : N5590-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

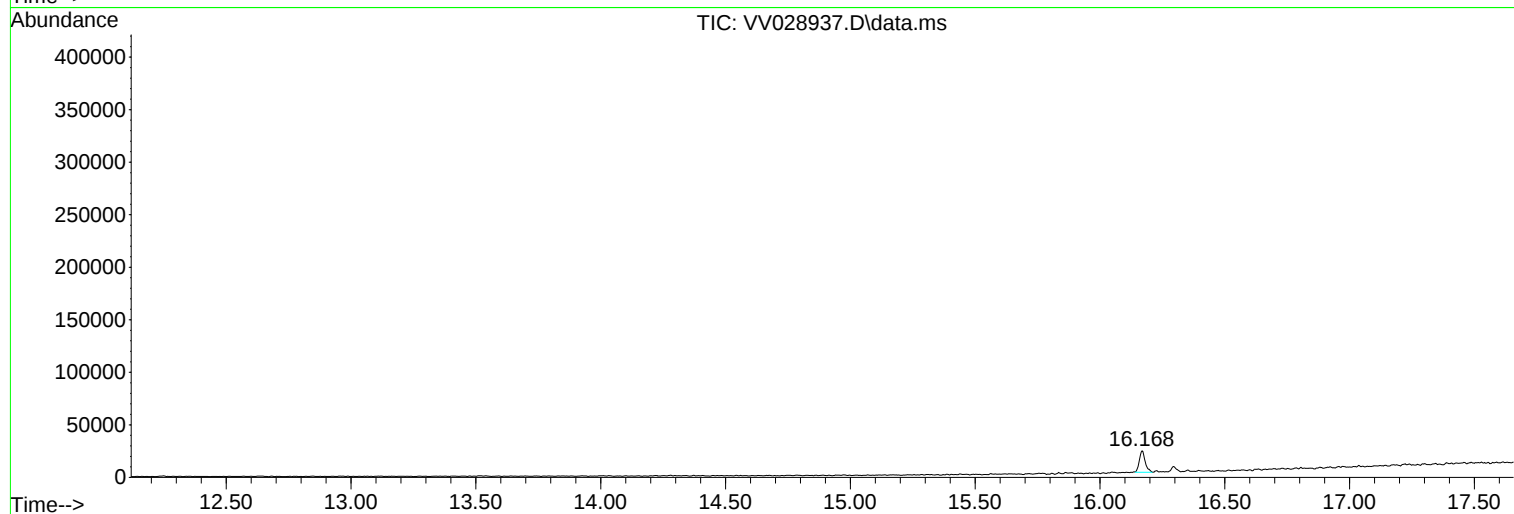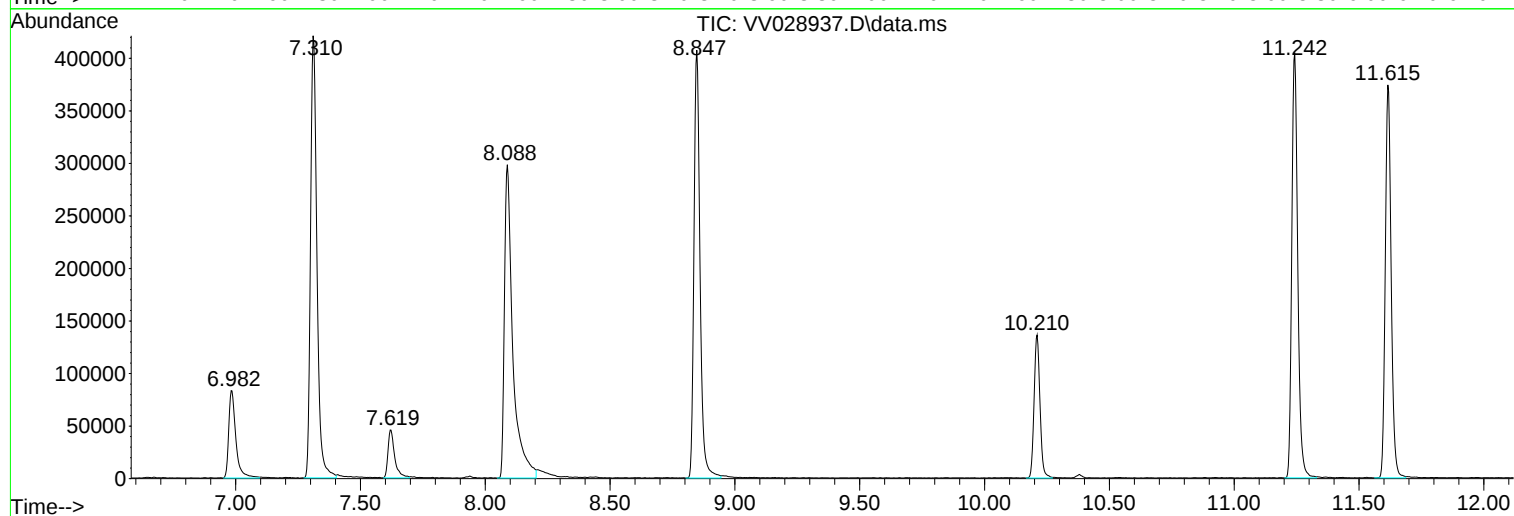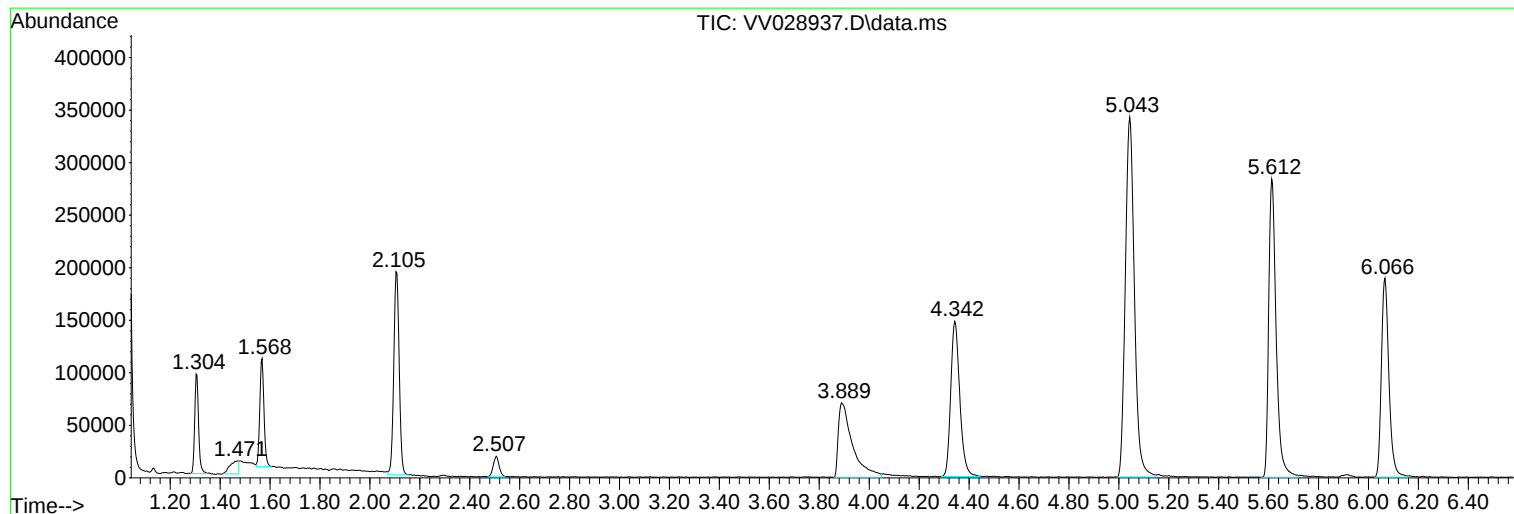

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028937.D
Acq On : 14 Nov 2022 14:45
Operator : SY/MD
Sample : N5590-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028937.D
Acq On : 14 Nov 2022 14:45
Operator : SY/MD
Sample : N5590-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc