

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028940.D
 Acq On : 14 Nov 2022 15:58
 Operator : SY/MD
 Sample : N5602-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	95	rBV2	110329	124869	14.63%	1.684%
2	1.420	110	118	122	rBV	25879	39205	4.59%	0.529%
3	1.568	157	164	177	rVB	98757	113502	13.30%	1.531%
4	2.108	321	332	348	rVB	188530	278278	32.61%	3.753%
5	3.905	875	891	941	rBV3	250874	764066	89.53%	10.304%
6	4.342	1011	1027	1052	rBV2	143108	362168	42.44%	4.884%
7	5.043	1229	1245	1283	rBV2	336483	853410	100.00%	11.509%
8	5.612	1411	1422	1450	rBV	282817	580309	68.00%	7.826%
9	5.924	1506	1519	1534	rVB7	4944	10922	1.28%	0.147%
10	6.066	1547	1563	1588	rBV	186439	388279	45.50%	5.236%
11	6.985	1838	1849	1872	rBV2	79470	156602	18.35%	2.112%
12	7.310	1939	1950	1986	rBV	401975	723439	84.77%	9.756%
13	7.622	2037	2047	2082	rBV2	42729	84833	9.94%	1.144%
14	8.088	2180	2192	2232	rBV	313715	712171	83.45%	9.604%
15	8.847	2415	2428	2453	rBV	408986	689240	80.76%	9.295%
16	10.210	2840	2852	2871	rBV	135318	222588	26.08%	3.002%
17	11.242	3161	3173	3194	rBV	415559	676747	79.30%	9.126%
18	11.615	3278	3289	3314	rBV	366022	614496	72.00%	8.287%
19	16.168	4697	4705	4717	rVB6	12624	20166	2.36%	0.272%




Sum of corrected areas: 7415290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028940.D
Acq On : 14 Nov 2022 15:58
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

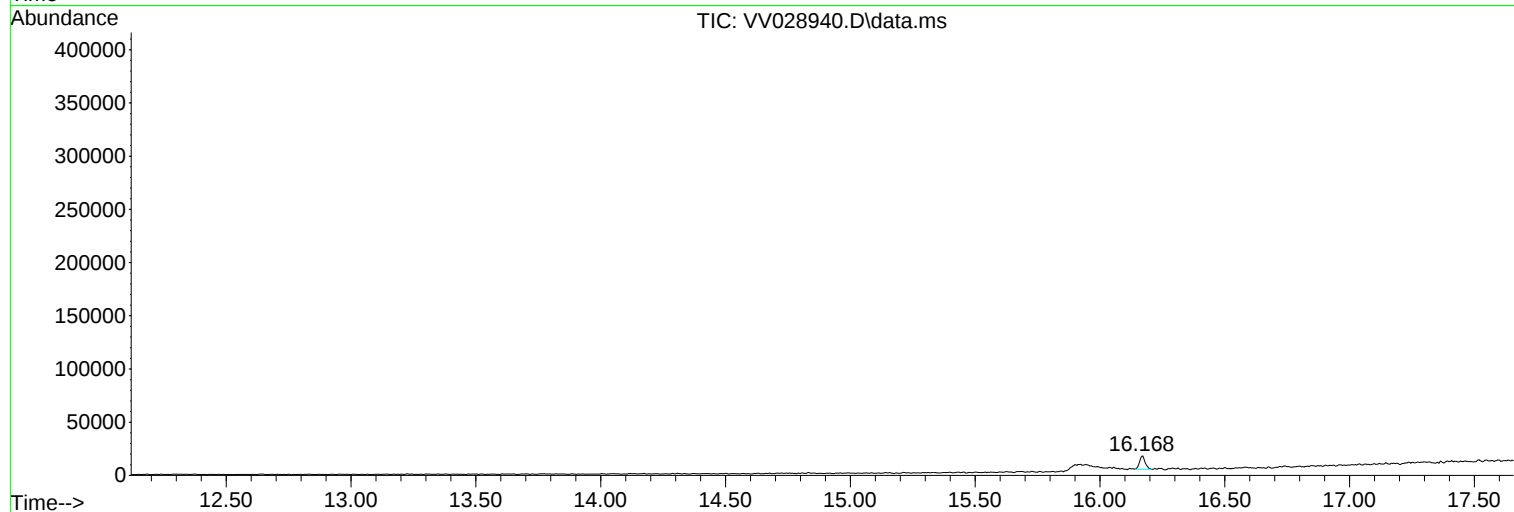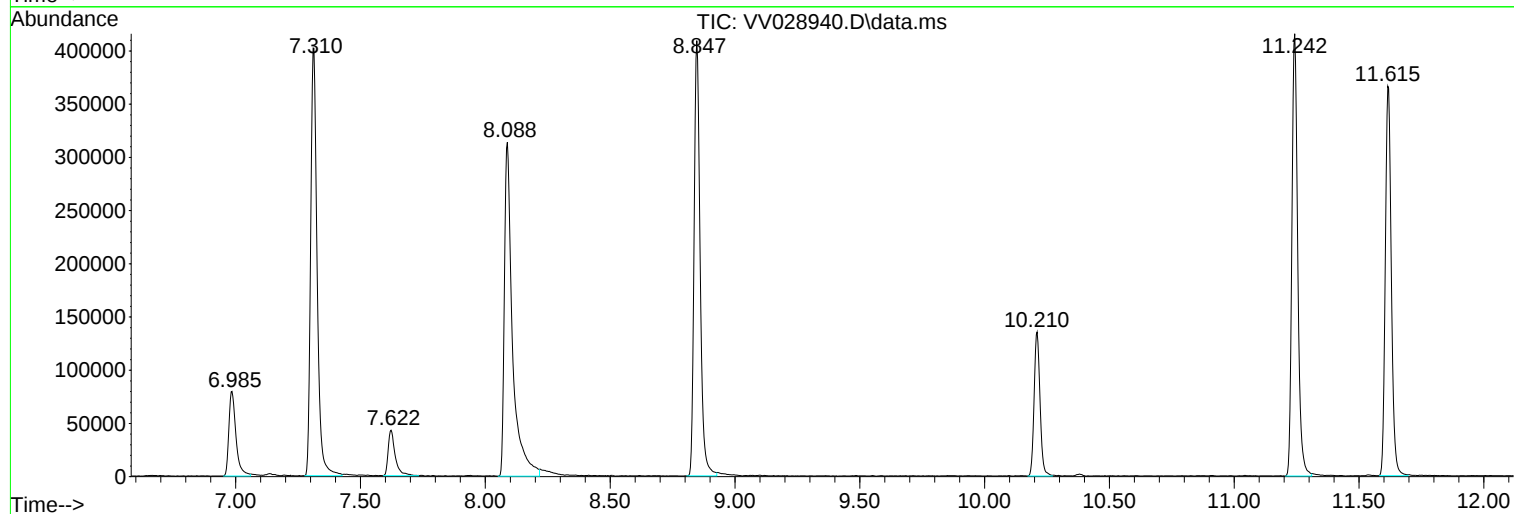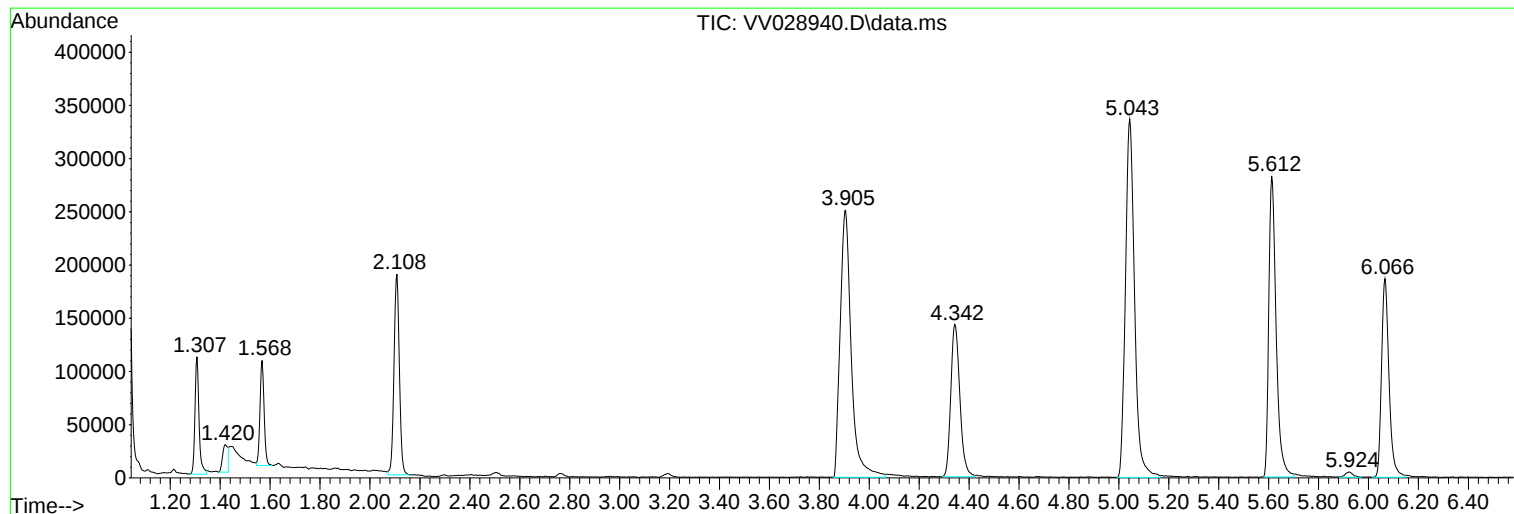

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028940.D
Acq On : 14 Nov 2022 15:58
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028940.D
Acq On : 14 Nov 2022 15:58
Operator : SY/MD
Sample : N5602-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc