

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028942.D
 Acq On : 14 Nov 2022 16:47
 Operator : SY/MD
 Sample : N5592-14DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AB9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	101	rBV	90368	100650	12.20%	1.274%
2	1.416	110	117	128	rBV2	24389	48337	5.86%	0.612%
3	1.568	157	164	174	rVB	94609	107626	13.05%	1.362%
4	2.108	322	332	350	rVB2	196508	304506	36.91%	3.854%
5	2.506	445	456	474	rBV	59531	100958	12.24%	1.278%
6	3.892	873	887	931	rBV4	95849	370017	44.85%	4.683%
7	4.346	1011	1028	1055	rBV2	139904	355433	43.08%	4.499%
8	5.043	1229	1245	1286	rBV2	325017	825004	100.00%	10.442%
9	5.612	1411	1422	1450	rBV	285117	586115	71.04%	7.419%
10	5.911	1504	1515	1545	rBV	130143	273487	33.15%	3.462%
11	6.066	1549	1563	1594	rVV	179394	379111	45.95%	4.799%
12	6.985	1837	1849	1873	rBV	76073	149948	18.18%	1.898%
13	7.313	1938	1951	1986	rBV	385666	709366	85.98%	8.979%
14	7.622	2038	2047	2070	rBV	42219	80707	9.78%	1.022%
15	7.969	2142	2155	2179	rBV	414820	695889	84.35%	8.808%
16	8.088	2182	2192	2238	rBV	296161	667837	80.95%	8.453%
17	8.847	2417	2428	2452	rBV	410316	700408	84.90%	8.865%
18	10.210	2841	2852	2873	rBV	128798	205275	24.88%	2.598%
19	11.242	3162	3173	3198	rBV	398916	656451	79.57%	8.309%
20	11.615	3278	3289	3312	rBV	344120	570585	69.16%	7.222%
21	16.168	4699	4705	4714	rVB	8394	12846	1.56%	0.163%




Sum of corrected areas: 7900556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028942.D
Acq On : 14 Nov 2022 16:47
Operator : SY/MD
Sample : N5592-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

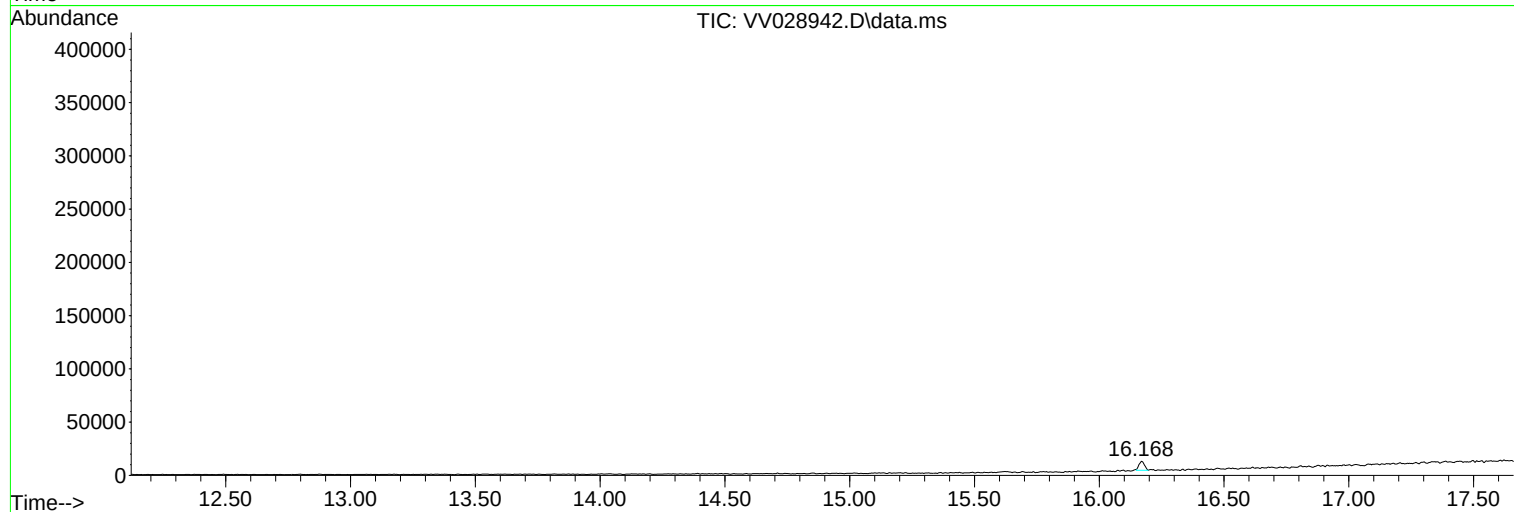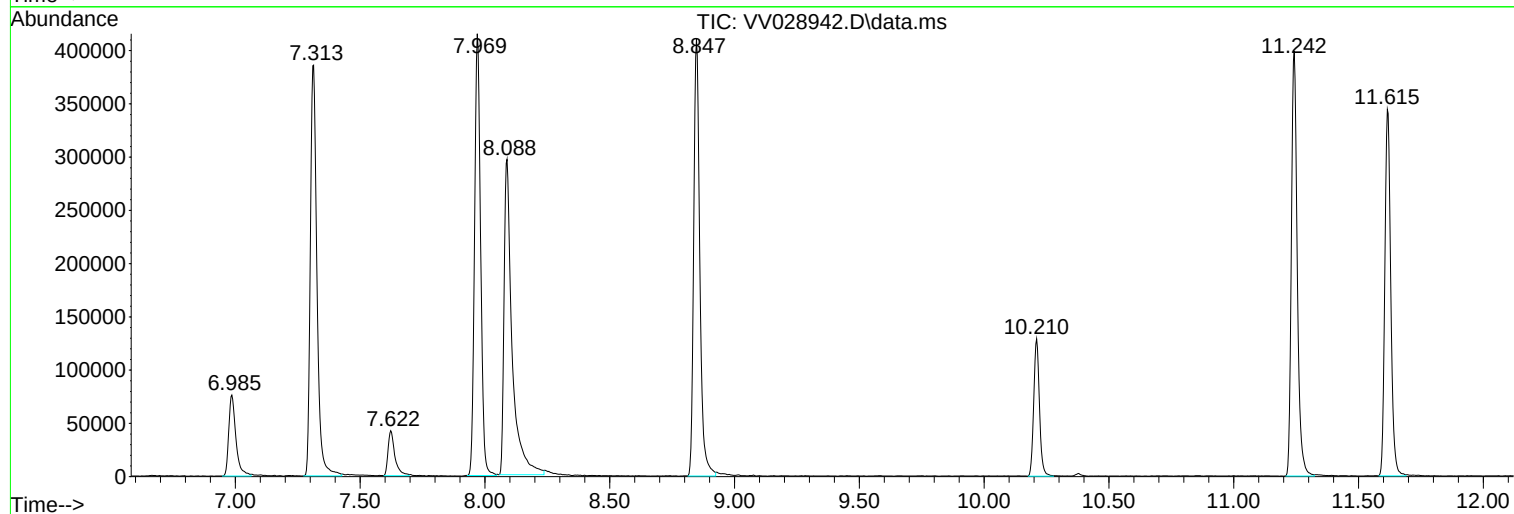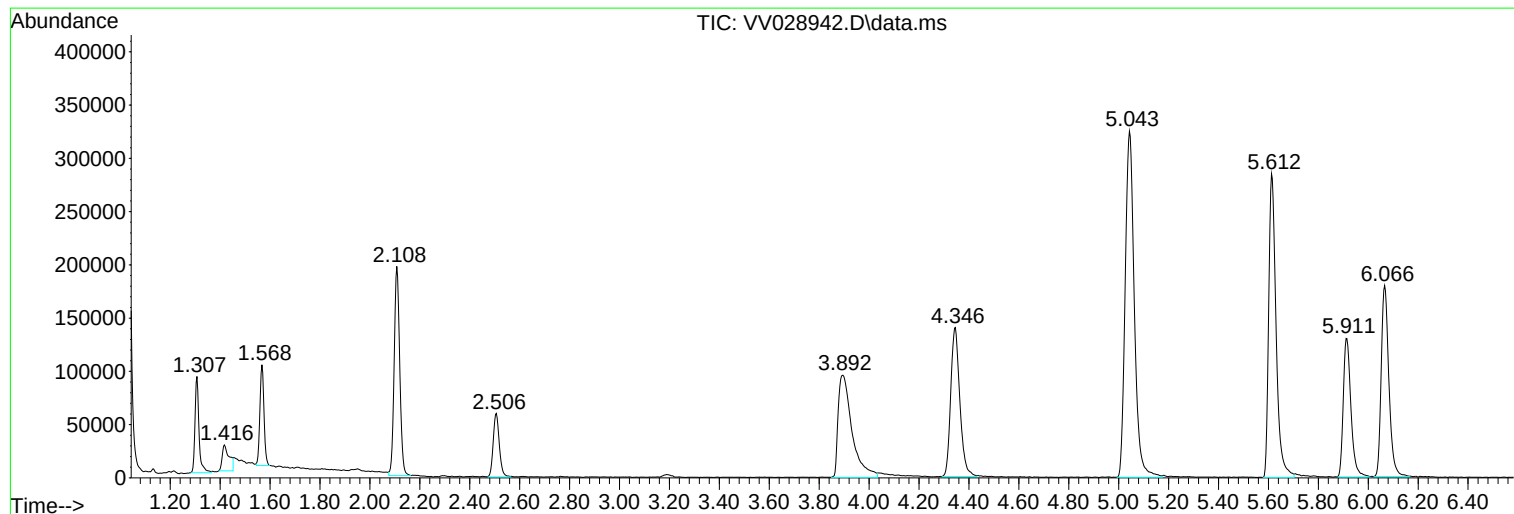

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028942.D
Acq On : 14 Nov 2022 16:47
Operator : SY/MD
Sample : N5592-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028942.D
Acq On : 14 Nov 2022 16:47
Operator : SY/MD
Sample : N5592-14DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc