

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028943.D
 Acq On : 14 Nov 2022 17:12
 Operator : SY/MD
 Sample : N5592-15DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rBV	91820	102081	12.07%	1.312%
2	1.416	110	117	121	rBV	25767	32243	3.81%	0.414%
3	1.568	157	164	176	rVB	99993	118099	13.96%	1.518%
4	2.108	322	332	349	rVB2	195597	291999	34.52%	3.754%
5	2.506	444	456	477	rVB	57365	96289	11.38%	1.238%
6	3.889	872	886	927	rBV2	90138	336071	39.73%	4.320%
7	4.342	1010	1027	1064	rVB	146436	368300	43.54%	4.735%
8	5.043	1229	1245	1271	rBV2	340510	845835	100.00%	10.874%
9	5.612	1409	1422	1453	rBV	271285	571589	67.58%	7.348%
10	5.915	1505	1516	1538	rBV2	77513	164079	19.40%	2.109%
11	6.066	1549	1563	1596	rBV2	187458	393039	46.47%	5.053%
12	6.985	1835	1849	1874	rBV	81607	157168	18.58%	2.020%
13	7.313	1937	1951	1990	rBV	405071	731817	86.52%	9.408%
14	7.622	2038	2047	2072	rBV2	43537	81478	9.63%	1.047%
15	7.969	2143	2155	2182	rBV2	395689	675050	79.81%	8.678%
16	8.088	2182	2192	2238	rBV	305322	693250	81.96%	8.912%
17	8.847	2417	2428	2456	rBV	399597	671692	79.41%	8.635%
18	10.210	2840	2852	2877	rBV	129799	214425	25.35%	2.757%
19	11.242	3161	3173	3205	rBV	382196	627981	74.24%	8.073%
20	11.615	3277	3289	3319	rBV	366473	592907	70.10%	7.622%
21	16.168	4696	4705	4714	rBV6	8695	13471	1.59%	0.173%




Sum of corrected areas: 7778863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028943.D
Acq On : 14 Nov 2022 17:12
Operator : SY/MD
Sample : N5592-15DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

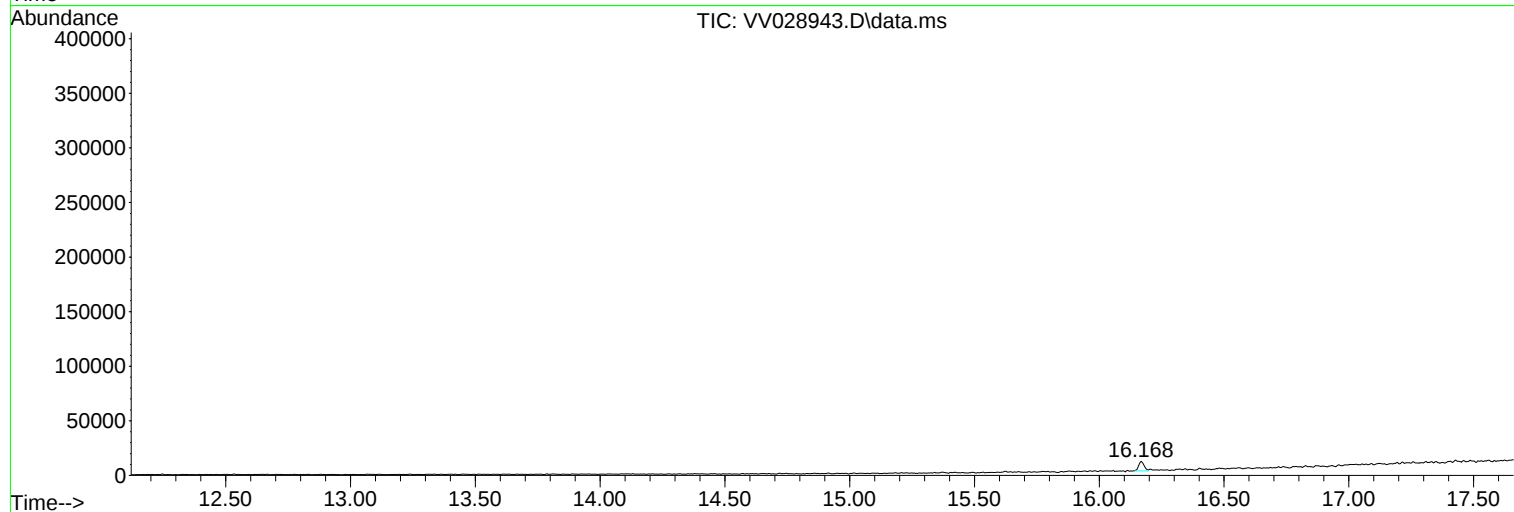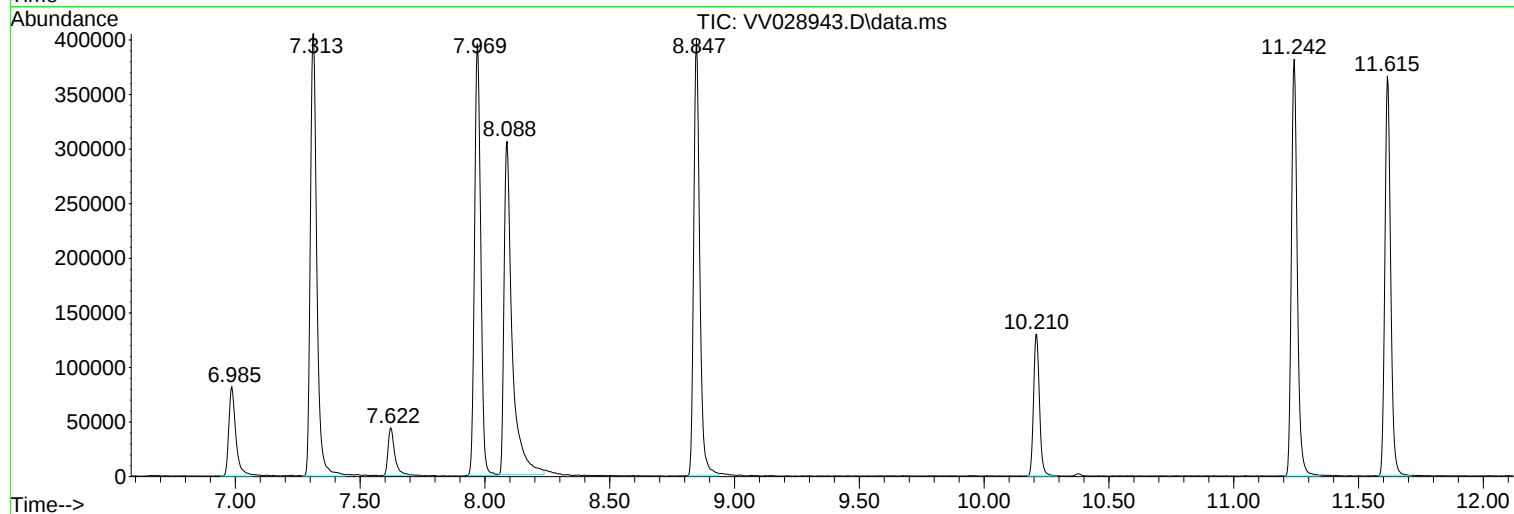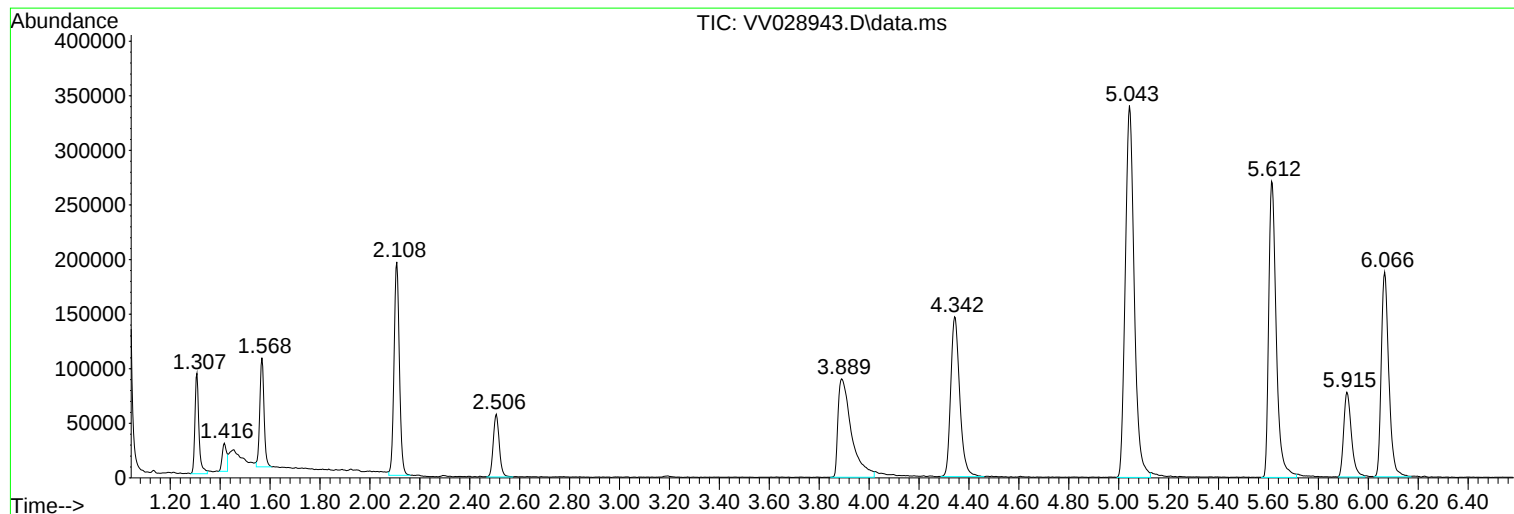

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028943.D
Acq On : 14 Nov 2022 17:12
Operator : SY/MD
Sample : N5592-15DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028943.D
Acq On : 14 Nov 2022 17:12
Operator : SY/MD
Sample : N5592-15DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc