

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028945.D
 Acq On : 14 Nov 2022 18:01
 Operator : SY/MD
 Sample : N5592-17DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rBV	94010	104098	11.68%	1.271%
2	1.416	109	117	122	rBV	18393	26488	2.97%	0.323%
3	1.568	157	164	182	rVB	103540	122555	13.75%	1.496%
4	2.108	322	332	350	rVB2	201120	300988	33.76%	3.674%
5	2.503	444	455	474	rBV	71707	120806	13.55%	1.475%
6	3.892	871	887	924	rBV2	88666	343247	38.50%	4.190%
7	4.342	1011	1027	1054	rBV	153368	388436	43.57%	4.742%
8	5.043	1229	1245	1277	rBV2	356256	891491	100.00%	10.883%
9	5.612	1408	1422	1449	rBV	303751	624170	70.01%	7.620%
10	5.915	1504	1516	1545	rBV2	79420	169073	18.97%	2.064%
11	6.066	1549	1563	1598	rBV	199008	414792	46.53%	5.064%
12	6.985	1839	1849	1871	rBV	84733	162695	18.25%	1.986%
13	7.310	1939	1950	1980	rBV	417660	762046	85.48%	9.303%
14	7.622	2037	2047	2068	rBV	46396	88936	9.98%	1.086%
15	7.969	2137	2155	2176	rBV	366353	621701	69.74%	7.590%
16	8.088	2182	2192	2236	rBV	337179	750581	84.19%	9.163%
17	8.847	2417	2428	2457	rBV	442645	742041	83.24%	9.059%
18	10.210	2841	2852	2878	rBV	151284	241883	27.13%	2.953%
19	11.242	3162	3173	3204	rBV	412451	678686	76.13%	8.285%
20	11.615	3278	3289	3313	rBV	389946	625368	70.15%	7.634%
21	16.171	4698	4706	4715	rBV9	6762	11502	1.29%	0.140%




Sum of corrected areas: 8191583

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028945.D
Acq On : 14 Nov 2022 18:01
Operator : SY/MD
Sample : N5592-17DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

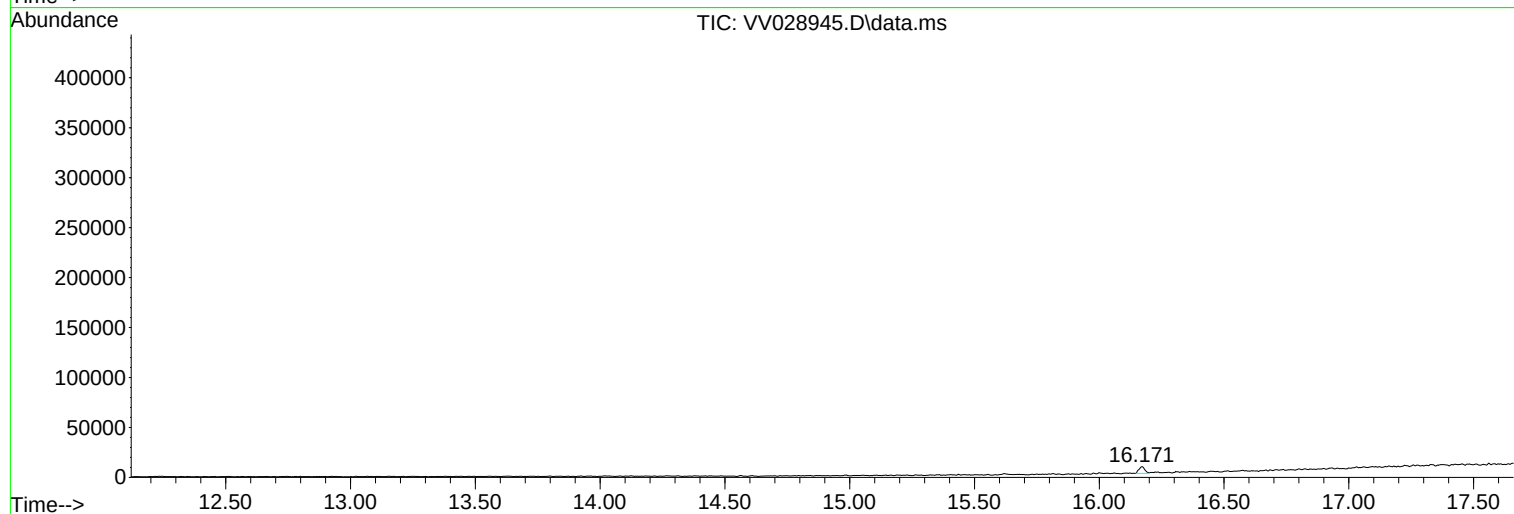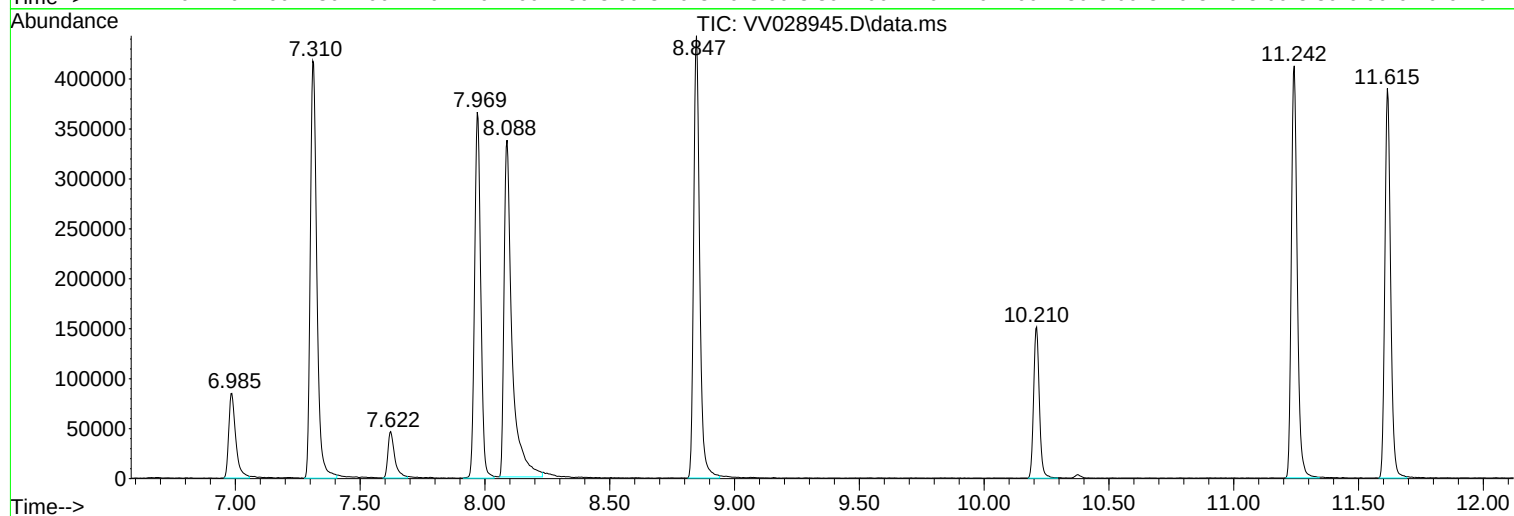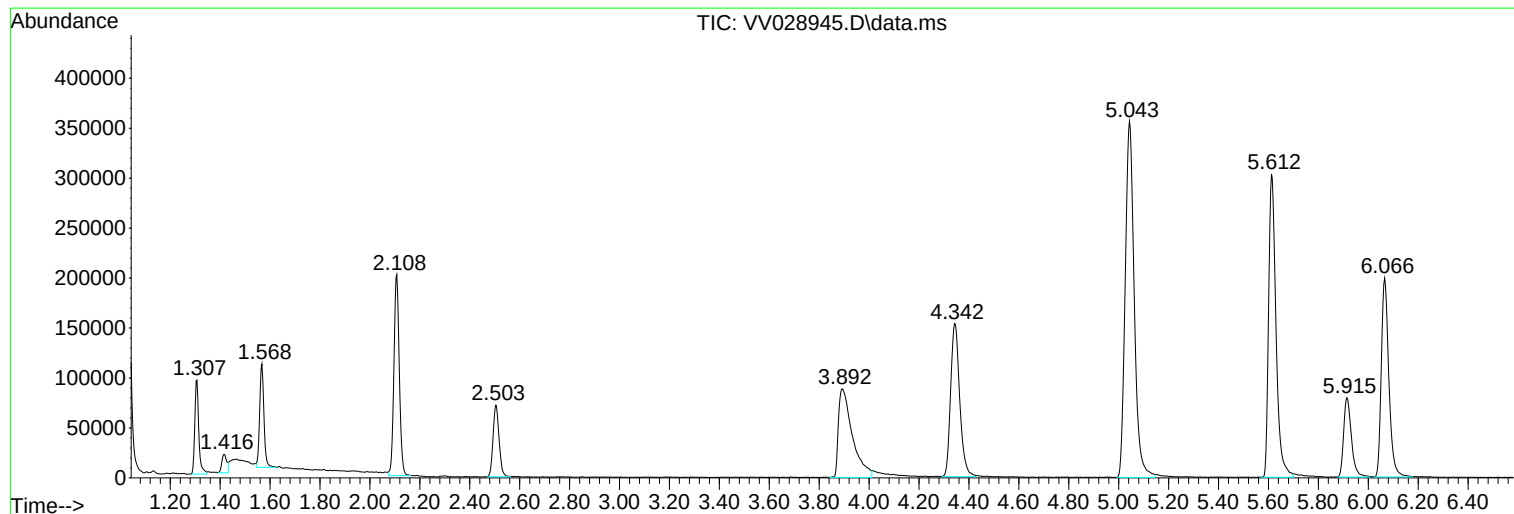

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028945.D
Acq On : 14 Nov 2022 18:01
Operator : SY/MD
Sample : N5592-17DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028945.D
Acq On : 14 Nov 2022 18:01
Operator : SY/MD
Sample : N5592-17DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc