

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
 Data File : VV028947.D
 Acq On : 14 Nov 2022 18:50
 Operator : SY/MD
 Sample : N5592-19DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rBV	88008	97407	11.57%	1.271%
2	1.458	121	130	132	rBV3	7304	10656	1.27%	0.139%
3	1.568	157	164	175	rVB	99346	114445	13.60%	1.493%
4	2.108	321	332	353	rVB2	191874	290908	34.56%	3.795%
5	2.506	445	456	474	rBV	82633	138476	16.45%	1.807%
6	3.899	873	889	927	rBV2	80398	329819	39.18%	4.303%
7	4.342	1010	1027	1059	rBV	143911	363199	43.15%	4.739%
8	5.043	1229	1245	1276	rBV2	333391	841753	100.00%	10.982%
9	5.612	1411	1422	1454	rBV	275978	579195	68.81%	7.557%
10	5.915	1504	1516	1545	rBV	84354	178873	21.25%	2.334%
11	6.066	1550	1563	1604	rVB	188907	391452	46.50%	5.107%
12	6.985	1837	1849	1873	rBV2	80448	156109	18.55%	2.037%
13	7.313	1939	1951	1978	rBV	398181	719406	85.47%	9.386%
14	7.622	2037	2047	2070	rBV	42582	81362	9.67%	1.062%
15	7.969	2132	2155	2177	rBV	306954	525533	62.43%	6.857%
16	8.088	2182	2192	2244	rBV	312077	722284	85.81%	9.424%
17	8.847	2416	2428	2458	rBV	409139	683922	81.25%	8.923%
18	10.210	2841	2852	2877	rBV	139534	225873	26.83%	2.947%
19	11.242	3162	3173	3203	rBV	386456	625236	74.28%	8.157%
20	11.615	3278	3289	3314	rBV	355890	588715	69.94%	7.681%




Sum of corrected areas: 7664623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028947.D
Acq On : 14 Nov 2022 18:50
Operator : SY/MD
Sample : N5592-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

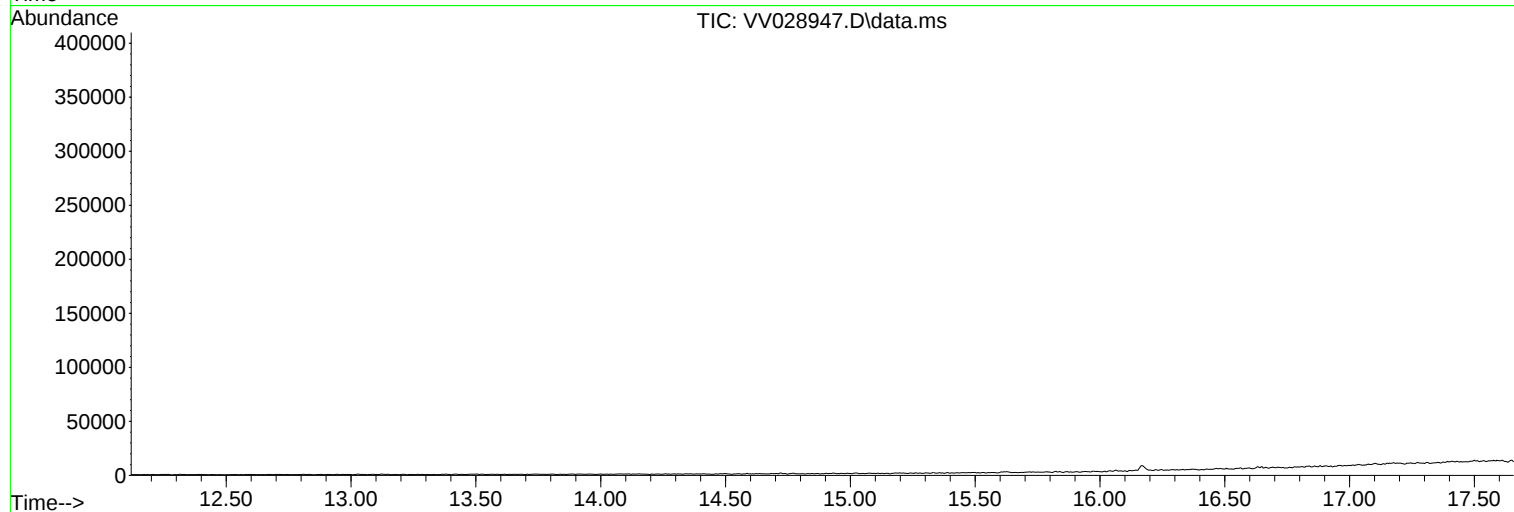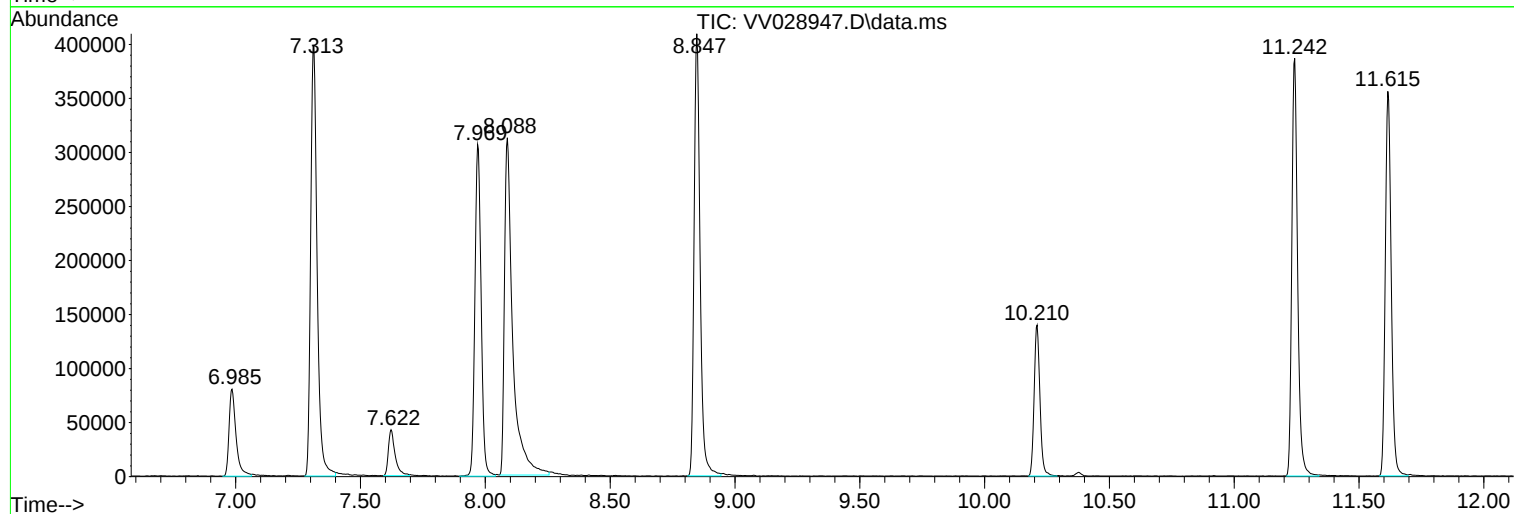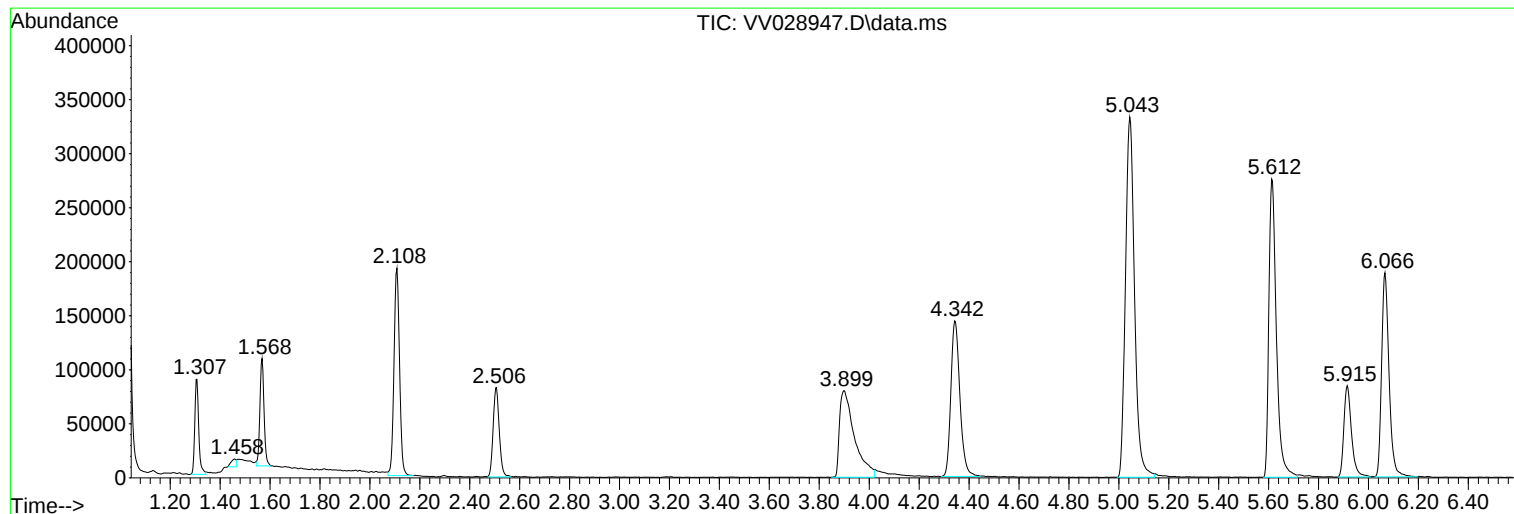

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028947.D
Acq On : 14 Nov 2022 18:50
Operator : SY/MD
Sample : N5592-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111422\
Data File : VV028947.D
Acq On : 14 Nov 2022 18:50
Operator : SY/MD
Sample : N5592-19DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc