


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111518\
Data File : VV008566.D
Acq On : 15 Nov 2018 11:06
Operator : SY/MD
Sample : BFB46
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111518WMA.M
Title : VOC Analysis
Last Update : Fri Nov 16 04:13:42 2018

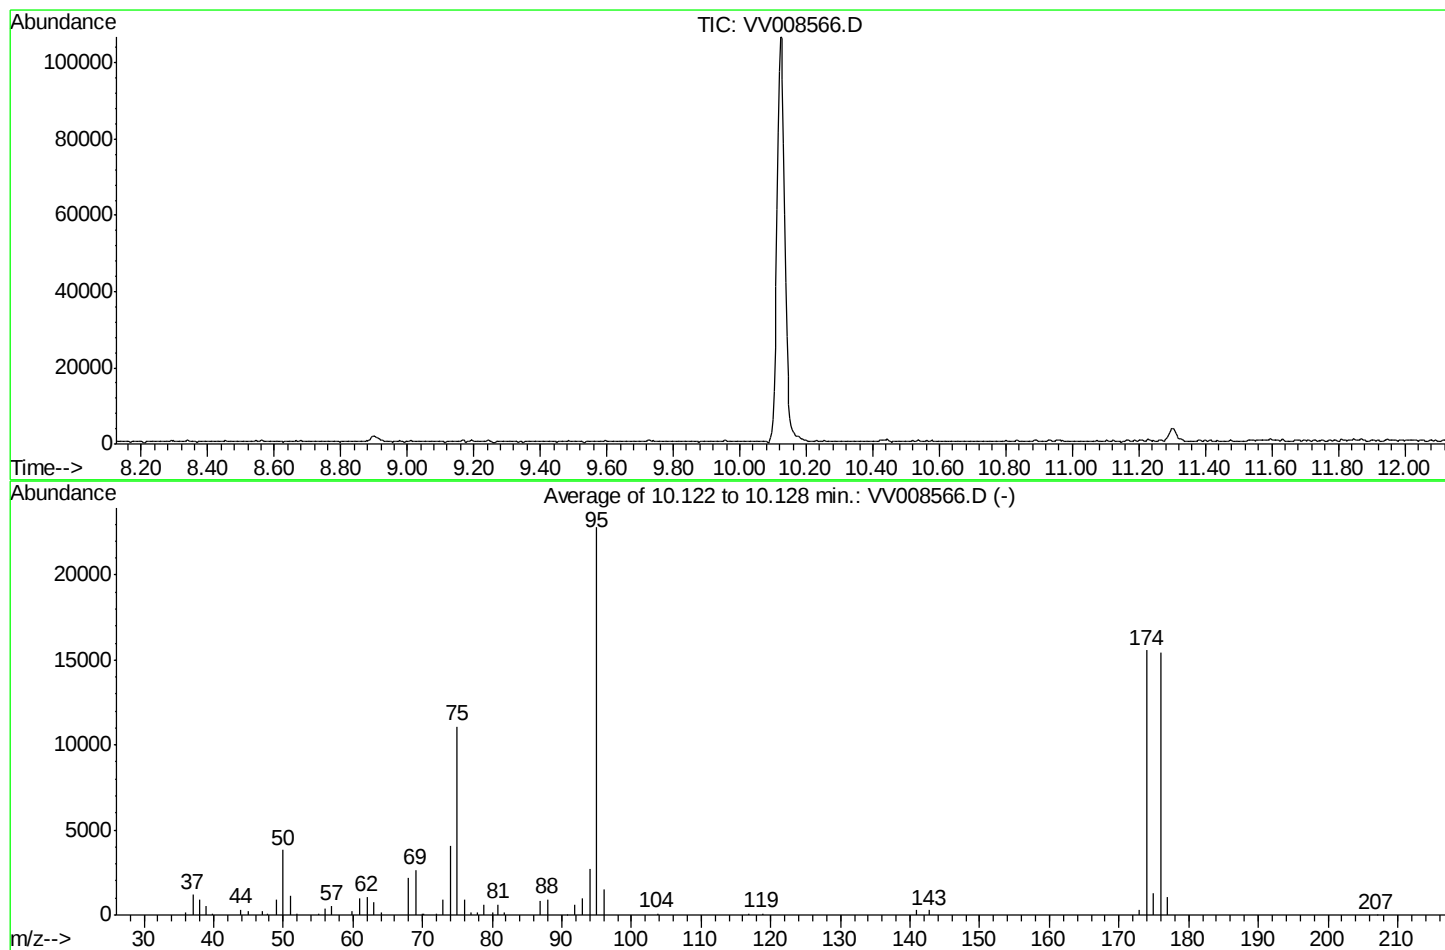

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	3808	PASS
75	95	30	80	48.7	11097	PASS
95	95	100	100	100.0	22802	PASS
96	95	5	9	6.6	1514	PASS
173	174	0.00	2	1.8	276	PASS
174	95	50	120	68.3	15571	PASS
175	174	5	9	8.0	1248	PASS
176	174	95	101	99.2	15452	PASS
177	176	5	9	6.9	1065	PASS

Scan 2797 (10.083 min): VV008566.D
BFB46

m/z	Abundance
40.00	127.0
43.90	386.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	188.0
37.00	1257.0
38.00	1046.0
38.90	478.0
39.90	161.0
43.90	748.0
45.00	255.0
47.00	229.0
47.80	124.0
49.00	943.0
50.00	3982.0
51.00	1209.0
51.90	116.0
55.00	140.0
56.00	425.0
56.90	635.0
59.90	186.0
61.00	1046.0
62.00	1198.0
63.00	853.0
64.00	159.0
68.00	2414.0
69.00	2619.0
69.90	138.0
71.90	133.0
73.00	855.0
74.00	4225.0
75.00	11530.0
76.00	953.0
76.90	195.0
77.90	181.0
78.90	667.0
80.00	232.0
80.90	651.0
81.80	211.0
87.00	923.0
87.90	863.0
91.90	623.0
92.90	1065.0
94.00	2803.0
95.00	23072.0
96.00	1572.0
103.70	130.0
116.80	115.0
118.80	175.0
140.90	280.0
142.80	276.0
173.00	278.0
174.00	16199.0
174.90	1268.0
176.00	15748.0
177.00	1058.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.10	170.0
37.10	1055.0
37.90	806.0
39.00	483.0
39.80	183.0
43.90	615.0
44.90	214.0
47.00	197.0
49.00	867.0
50.00	3595.0
51.00	1016.0
56.00	278.0
57.10	490.0
60.00	290.0
61.00	902.0
62.00	878.0
63.00	621.0
64.00	174.0
68.00	1988.0
69.00	2503.0
70.10	160.0
73.00	887.0
74.00	3767.0
75.00	10282.0
76.00	864.0
77.10	124.0
77.90	145.0
78.80	525.0
80.00	146.0
80.90	567.0
81.80	166.0
86.90	682.0
88.00	951.0
91.90	607.0
92.90	820.0
94.00	2451.0
95.00	21824.0
96.00	1407.0
140.80	249.0
142.80	270.0
172.90	265.0
174.00	14439.0
174.90	1183.0
176.00	14641.0
176.90	1060.0
207.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	195.0
37.10	1236.0
37.90	959.0
39.00	522.0
39.80	171.0
43.90	721.0
44.90	227.0
47.00	225.0
47.80	116.0
49.00	955.0
50.00	3847.0
51.00	1151.0
51.90	119.0
55.00	126.0
56.00	388.0
57.00	560.0
59.90	243.0
61.00	1046.0
62.00	1098.0
63.00	780.0
64.00	174.0
68.00	2269.0
69.00	2825.0
70.10	146.0
71.90	111.0
73.00	869.0
74.00	4169.0
75.00	11480.0
76.00	931.0
77.00	141.0
77.90	180.0
78.80	674.0
80.00	187.0
80.90	592.0
81.80	184.0
86.90	827.0
87.90	965.0
90.80	111.0
91.90	633.0
92.90	1006.0
94.00	2784.0
95.00	23512.0
96.00	1565.0
103.70	110.0
116.70	103.0
118.90	147.0
140.90	288.0
142.80	290.0
173.00	286.0
174.00	16076.0
175.00	1293.0
176.00	15967.0
177.00	1077.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46