

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111519\
 Data File : VV013642.D
 Acq On : 15 Nov 2019 16:32
 Operator : SY/MD
 Sample : VV1115WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK55

Quant Time: Nov 16 00:10:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 15 23:49:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	398966	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	389909	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	172770	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	114785	4.66	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.20%
7) Chloroethane-d5	1.58	69	103284	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.13	63	154811	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.96	46	273084	47.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.84%
24) Chloroform-d	4.40	84	249459	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
26) 1,2-Dichloroethane-d4	5.08	65	124093	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.80%
32) Benzene-d6	5.09	84	499062	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	6.11	67	152770	4.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.20%
41) Toluene-d8	7.36	98	440119	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.66	79	53698	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.14	63	207316	44.32	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.64%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	103582	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	171026	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	6755	0.204 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111519\
Data File : VV013642.D
Acq On : 15 Nov 2019 16:32
Operator : SY/MD
Sample : VV1115WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK55

Quant Time: Nov 16 00:10:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 15 23:49:05 2019
Response via : Initial Calibration

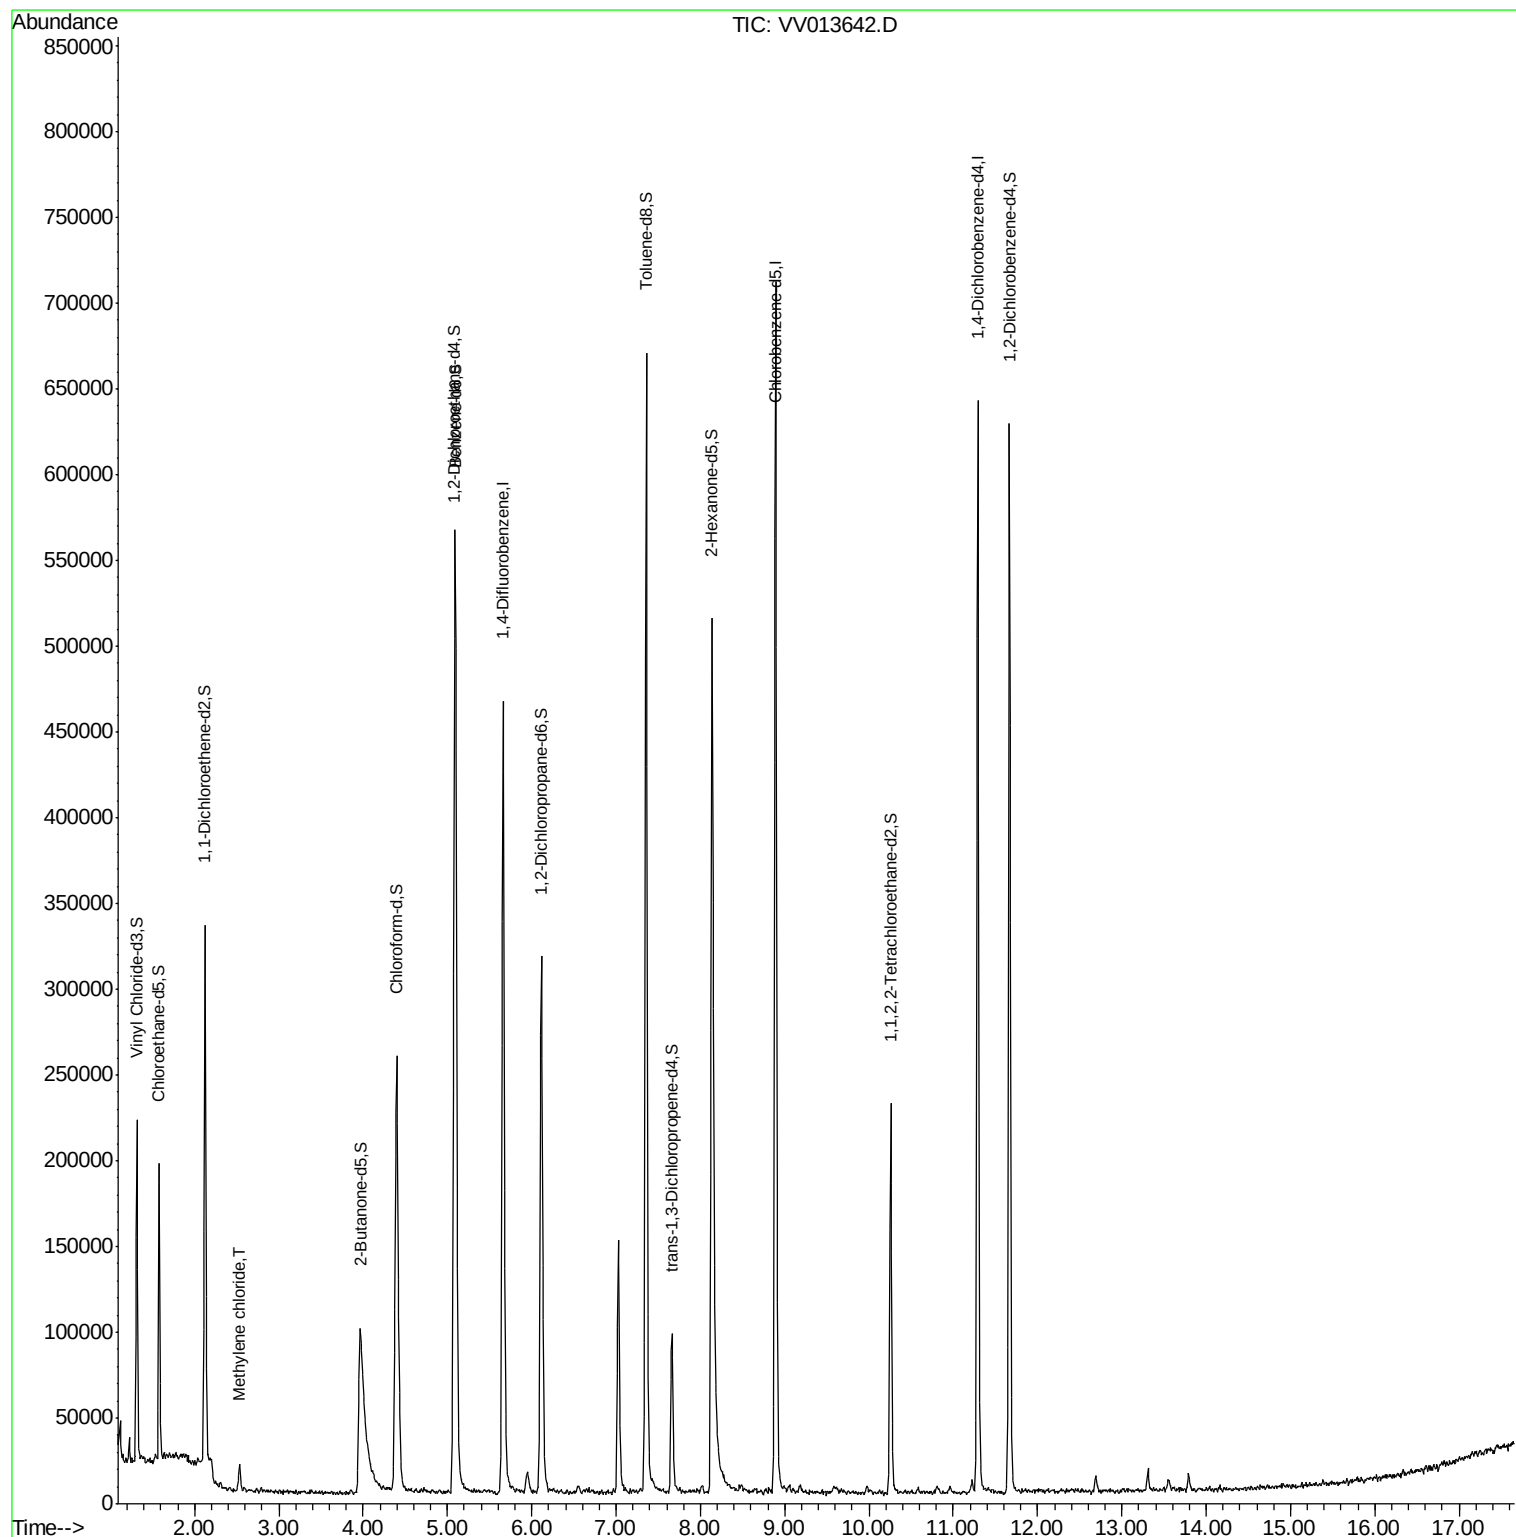

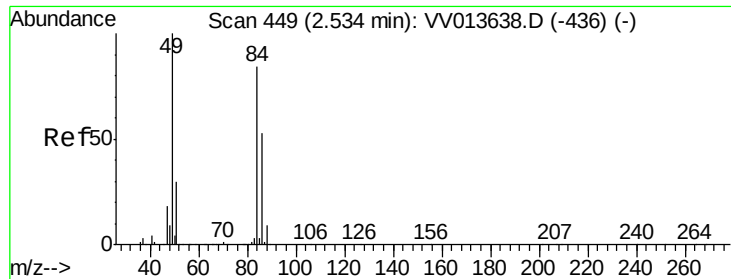

#16
 Methvlene chloride
 Concen: 0.204 ug/L
 RT: 2.53 min Scan# 449
 Delta R.T. -0.00 min
 Lab File: VV013642.D
 Acq: 15 Nov 2019 16:32

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK55

Tot Ion	Ratio	Lower	Upper
84	100		
86	66.7	44.1	81.9
49	127.2	83.4	155.0

