


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023471.D
Acq On : 15 Nov 2021 10:33
Operator : SY/MD
Sample : VV1115WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK252

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:30:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 16 00:29:25 2021
Response via : Initial Calibration

Reviewed By : John Carlone 11/16/2021
Supervised By : Mahesh Dadoda 11/16/2021

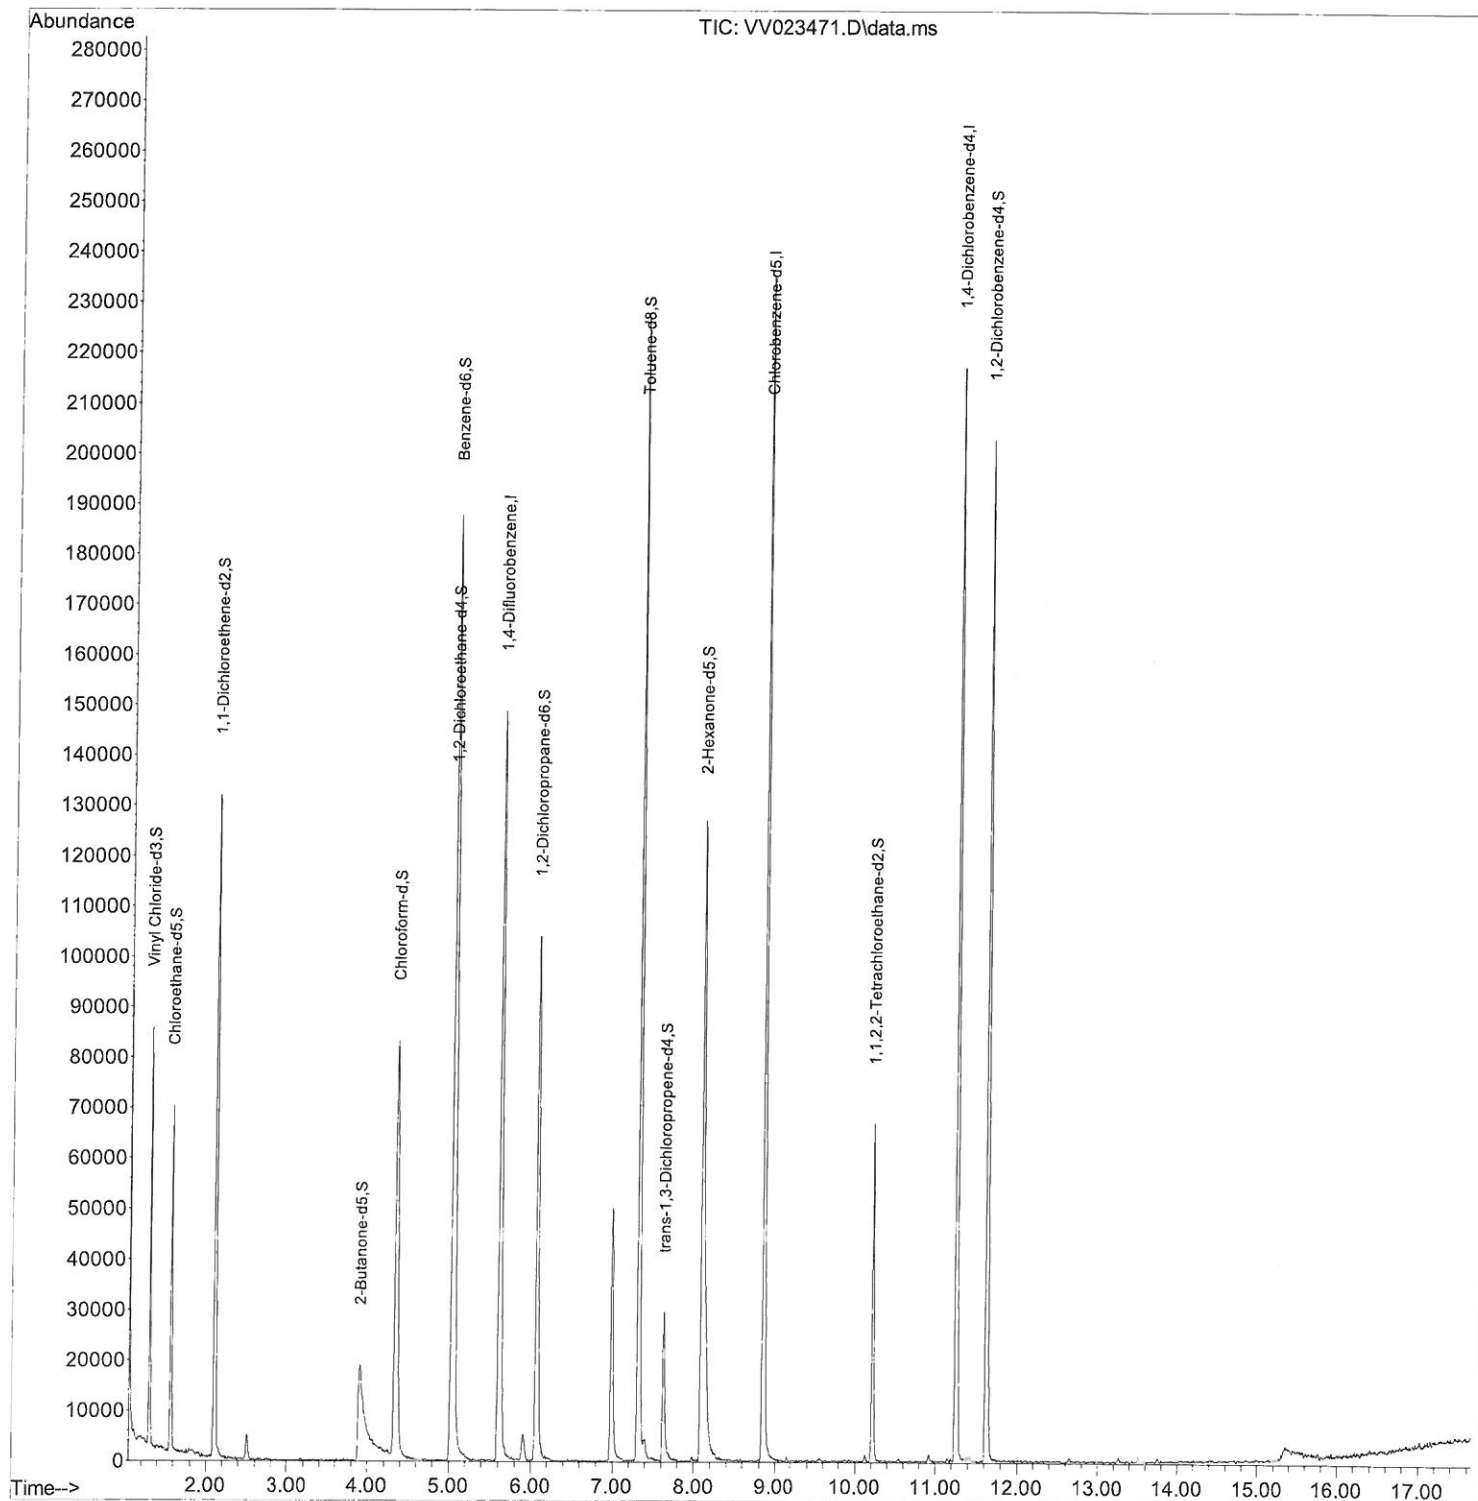

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023471.D
 Acq On : 15 Nov 2021 10:33
 Operator : SY/MD
 Sample : VV1115WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 VBLK252

Manual Integrations APPROVED

Quant Time: Nov 16 00:30:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 16 00:29:25 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 11/16/2021
 Supervised By : Mahesh Dadoda 11/16/2021

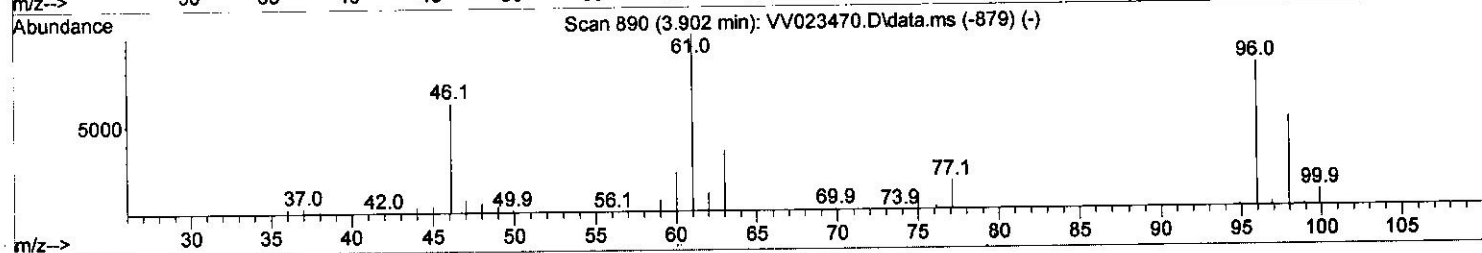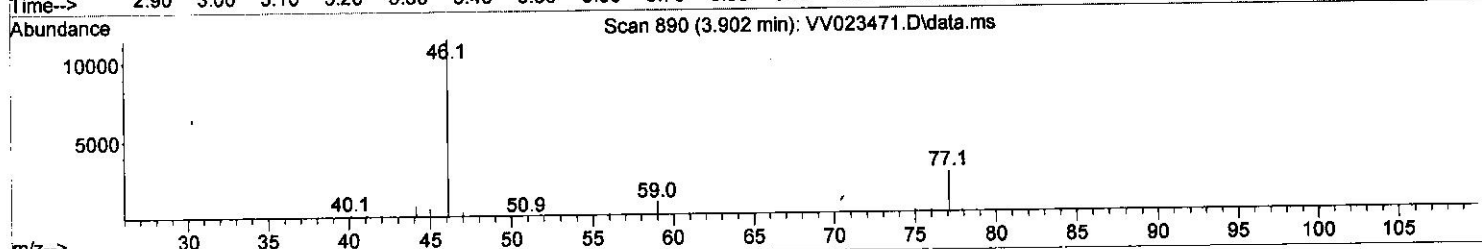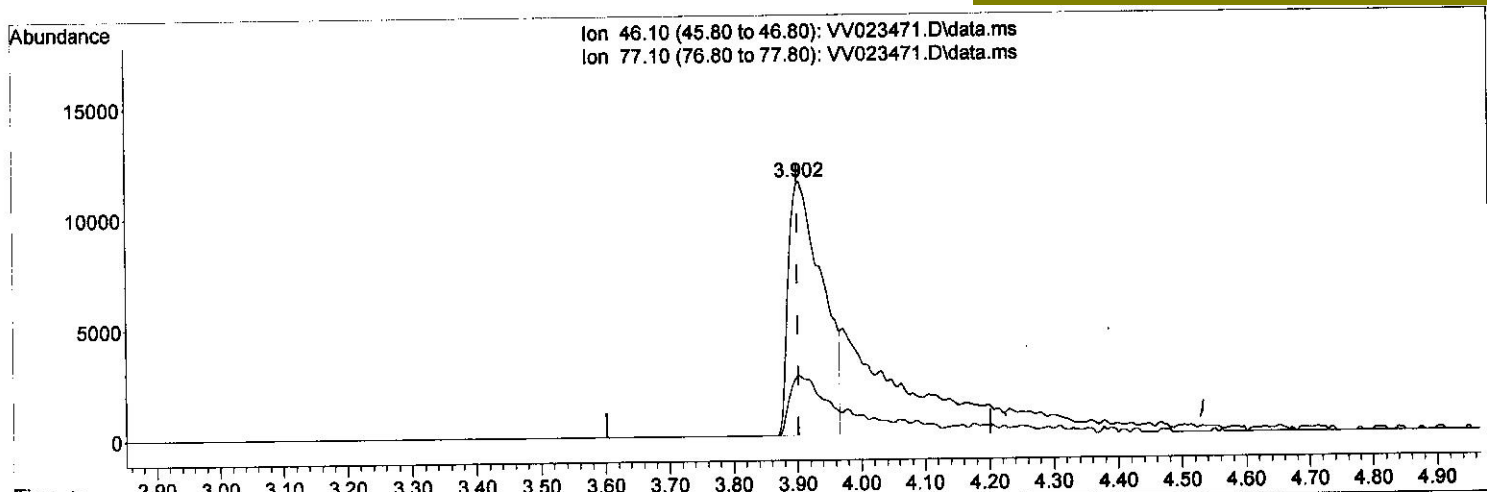

TIC: VV023471.D\data.ms

(20) 2-Butanone-d5 (S)

3.902min (+ 0.000) 29.44 ug/L

response 42227

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	24.79
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023471.D
 Acq On : 15 Nov 2021 10:33
 Operator : SY/MD
 Sample : VV1115WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK252

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:30:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 16 00:29:25 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/16/2021
 Supervised By :Mahesh Dadoda 11/16/2021

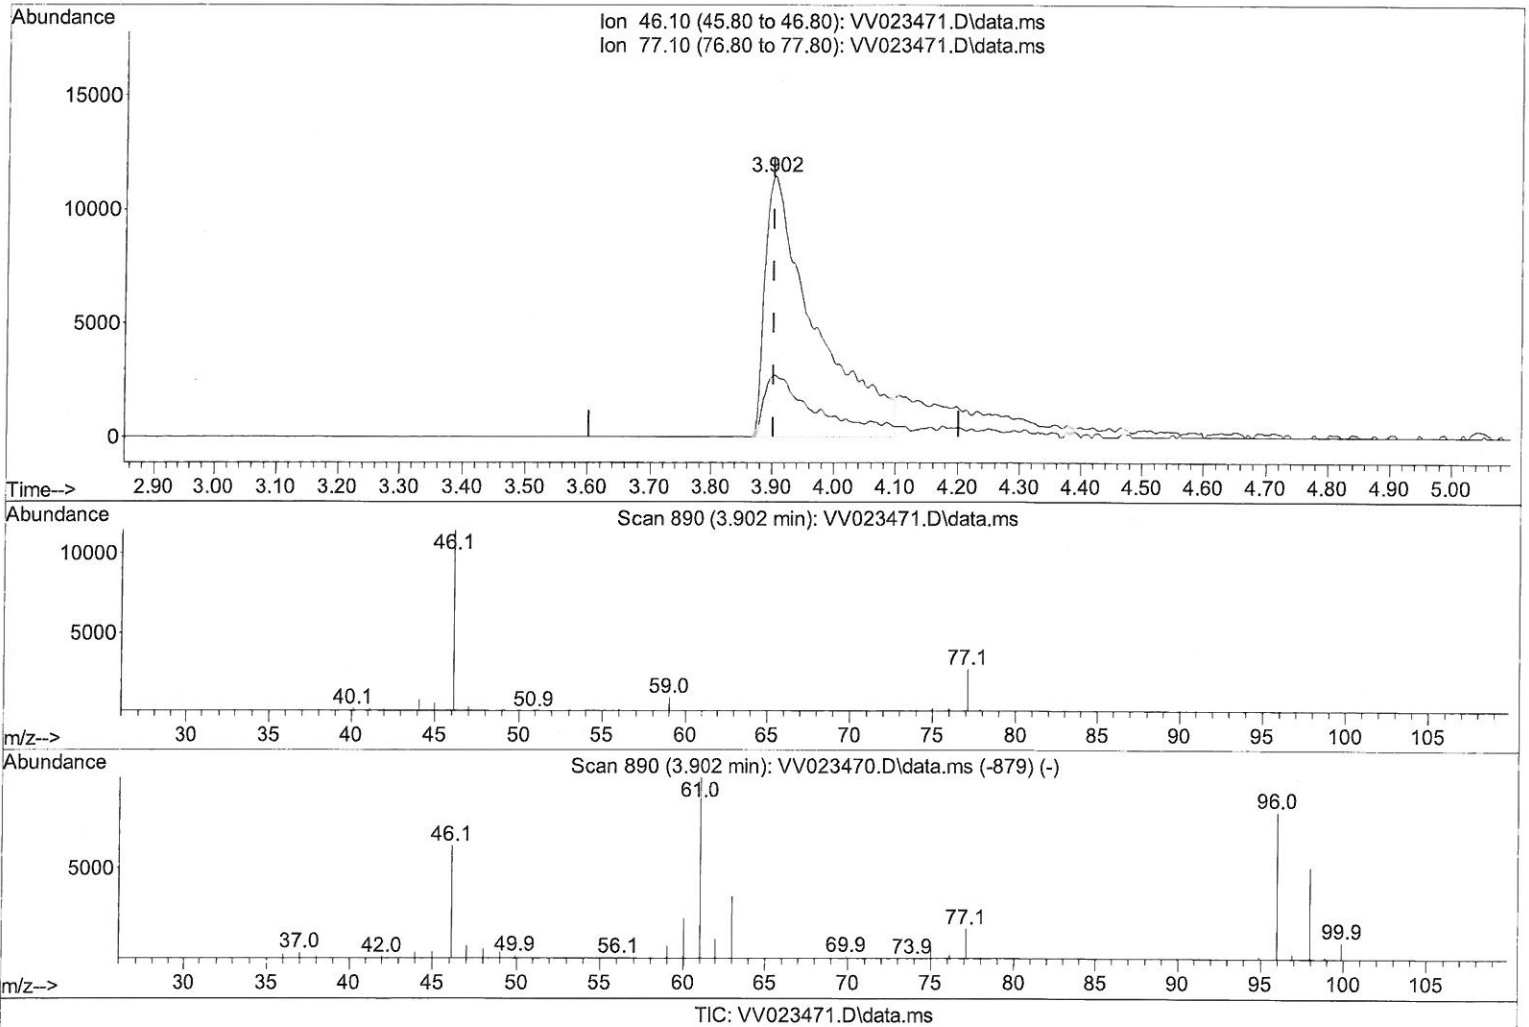

(20) 2-Butanone-d5 (S)

3.902min (+ 0.000) 44.96 ug/L m

response 64488

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	16.23
0.00	0.00	0.00
0.00	0.00	0.00

MD
 11/22/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023471.D
 Acq On : 15 Nov 2021 10:33
 Operator : SY/MD
 Sample : VV1115WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sample Id :
 VBLK252

Manual Integrations APPROVED

Reviewed By : John Carlone 11/16/2021
 Supervised By : Mahesh Dadoda 11/16/2021

Quant Time: Nov 16 00:30:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 16 00:29:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	132890	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	134107	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61038	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	51847	6.228	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 124.600%			
7) Chloroethane-d5	1.565	69	40053	5.903	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 118.000%			
11) 1,1-Dichloroethene-d2	2.101	63	68336	4.385	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 87.600%			
20) 2-Butanone-d5	3.902	46	64488m	44.963	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 89.920%			
24) Chloroform-d	4.343	84	88125	4.967	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 99.400%			
26) 1,2-Dichloroethane-d4	5.027	65	41406	5.190	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 103.800%			
32) Benzene-d6	5.043	84	173741	5.049	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 101.000%			
36) 1,2-Dichloropropane-d6	6.066	67	51071	5.042	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 100.800%			
41) Toluene-d8	7.313	98	151191	4.689	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 93.800%			
43) trans-1,3-Dichloroprop...	7.622	79	18897	4.920	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 98.400%			
46) 2-Hexanone-d5	8.088	63	50981	36.077	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 72.160%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31809	4.367	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 87.400%			
66) 1,2-Dichlorobenzene-d4	11.622	152	55311	5.442	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 108.800%			

MD
11/22/21

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed