

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111521\
 Data File : VW023509.D
 Acq On : 16 Nov 2021 01:55
 Operator : SY/MD
 Sample : M4694-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4634

Quant Time: Nov 16 05:17:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 16 02:06:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124543	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124722	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55234	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	39061	5.006	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.571	69	33028	5.194	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.800%	
11) 1,1-Dichloroethene-d2	2.111	63	53083	3.634	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.600%	
20) 2-Butanone-d5	3.895	46	70202	52.227	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.460%	
24) Chloroform-d	4.349	84	74663	4.490	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.800%	
26) 1,2-Dichloroethane-d4	5.037	65	36188	4.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.800%	
32) Benzene-d6	5.053	84	144854	4.527	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.600%	
36) 1,2-Dichloropropane-d6	6.069	67	43195	4.585	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.800%	
41) Toluene-d8	7.317	98	125665	4.191	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	7.625	79	14754	4.130	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.600%	
46) 2-Hexanone-d5	8.091	63	41115	31.284	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	62.560%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24007	3.544	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	70.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	47023	5.113	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.200%	
Target Compounds					Qvalue	
13) Acetone	2.185	43	8787	10.699	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023509.D
Acq On : 16 Nov 2021 01:55
Operator : SY/MD
Sample : M4694-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4634


Quant Time: Nov 16 05:17:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 16 02:06:43 2021
Response via : Initial Calibration

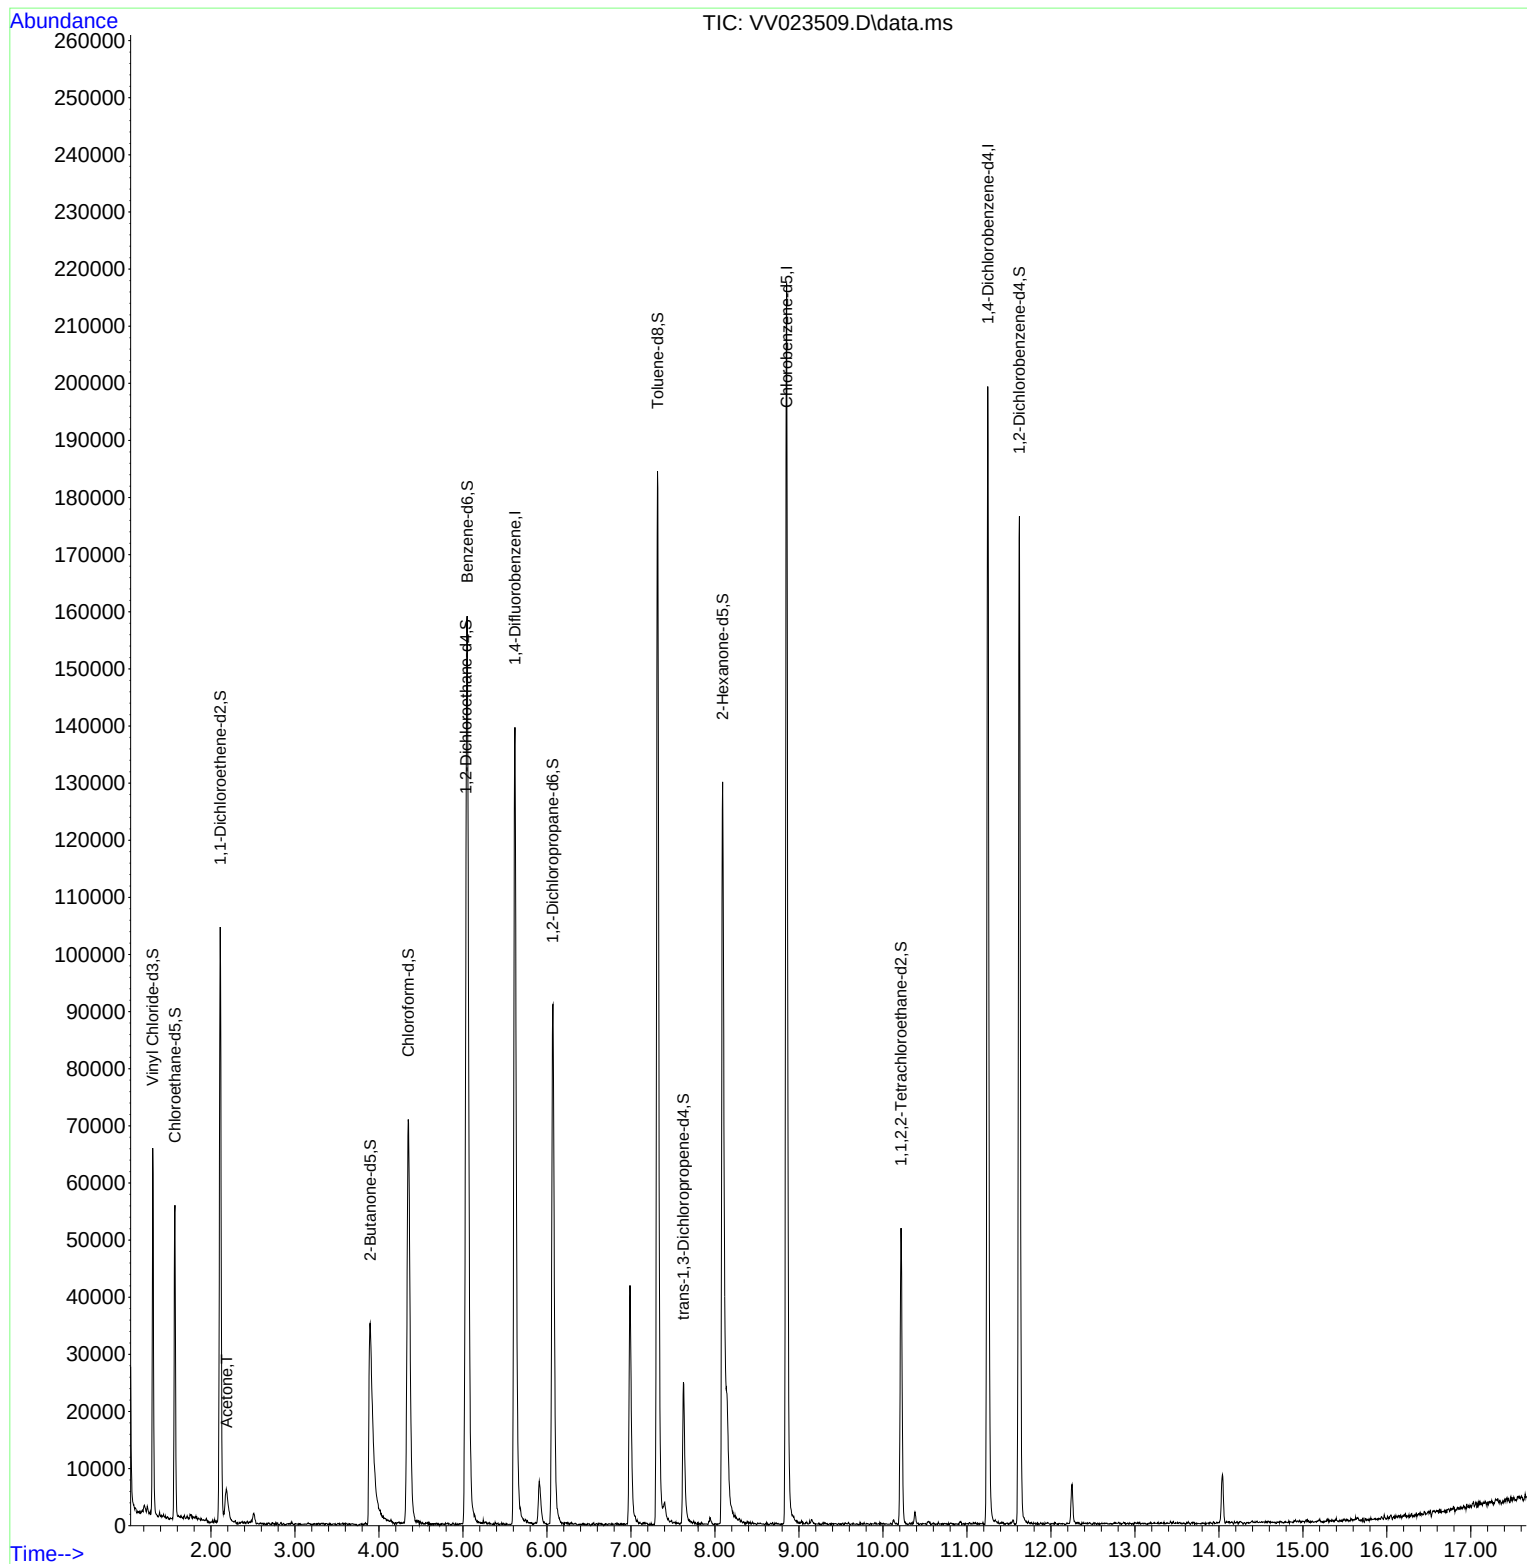


Abundance Scan 355 (2.182 min): VV023495.D\data.ms (-34

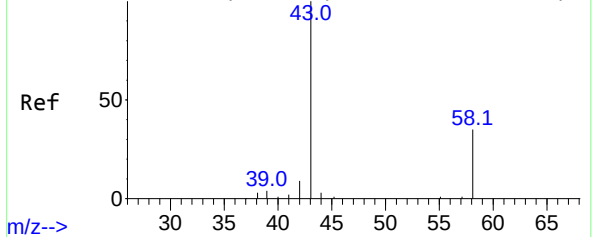

Abundance Scan 356 (2.185 min): VV023509.D\data.ms

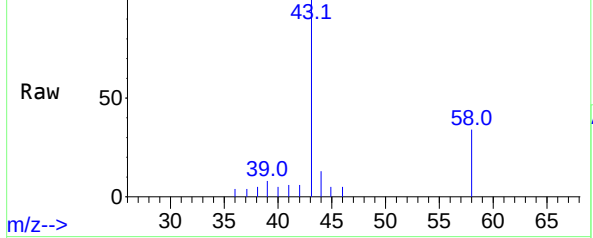

Abundance Scan 356 (2.185 min): VV023509.D\data.ms (-26

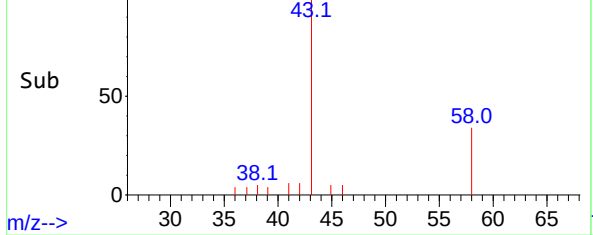

#13

Acetone

Concen: 10.699 ug/L

RT: 2.185 min Scan# 3

Delta R.T. 0.003 min

Lab File: VV023509.D

Acq: 16 Nov 2021 01:55

Instrument :

MSVOA_V

ClientSampleId :

H4634

Tgt Ion: 43 Resp: 8787

Ion Ratio Lower Upper

43 100

58 34.2 0.0 55.4

Abundance

