

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023472.D
 Acq On : 15 Nov 2021 11:09
 Operator : SY/MD
 Sample : M4616-04DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1X7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	59	rBV	131815	114370	17.16%	2.690%
2	1.307	75	83	98	rVB	76818	80136	12.03%	1.885%
3	1.568	156	164	174	rBV	60598	66960	10.05%	1.575%
4	1.754	211	222	243	rBV	505068	666402	100.00%	15.674%
5	2.108	320	332	351	rBV	126150	192144	28.83%	4.519%
6	2.507	443	456	468	rBV2	13869	23349	3.50%	0.549%
7	3.191	658	669	685	rVB	3640	7152	1.07%	0.168%
8	3.905	878	891	918	rBV3	25672	105693	15.86%	2.486%
9	4.342	1012	1027	1052	rBV2	75641	189171	28.39%	4.449%
10	5.043	1227	1245	1273	rBV2	170259	423948	63.62%	9.972%
11	5.613	1408	1422	1446	rBV	139508	289822	43.49%	6.817%
12	5.912	1503	1515	1532	rBV6	17941	40767	6.12%	0.959%
13	6.066	1549	1563	1585	rBV2	94972	197400	29.62%	4.643%
14	6.985	1836	1849	1866	rBV	44743	84535	12.69%	1.988%
15	7.313	1939	1951	1971	rBV	203133	356746	53.53%	8.391%
16	7.622	2037	2047	2066	rBV2	26260	49267	7.39%	1.159%
17	8.091	2182	2193	2224	rBV2	125065	299242	44.90%	7.038%
18	8.850	2416	2429	2446	rBV	219668	359143	53.89%	8.447%
19	10.217	2842	2854	2869	rBV	58700	94621	14.20%	2.226%
20	11.249	3162	3175	3194	rBV	204975	318622	47.81%	7.494%
21	11.625	3281	3292	3309	rBV	182196	292045	43.82%	6.869%




Sum of corrected areas: 4251535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023472.D
Acq On : 15 Nov 2021 11:09
Operator : SY/MD
Sample : M4616-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

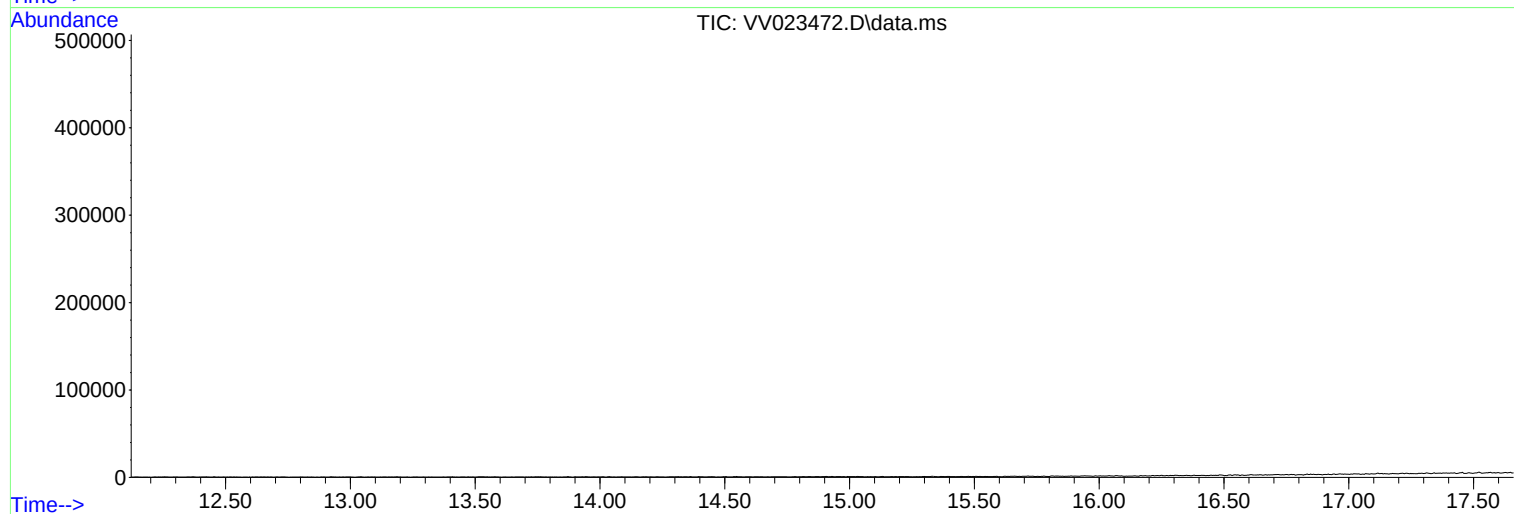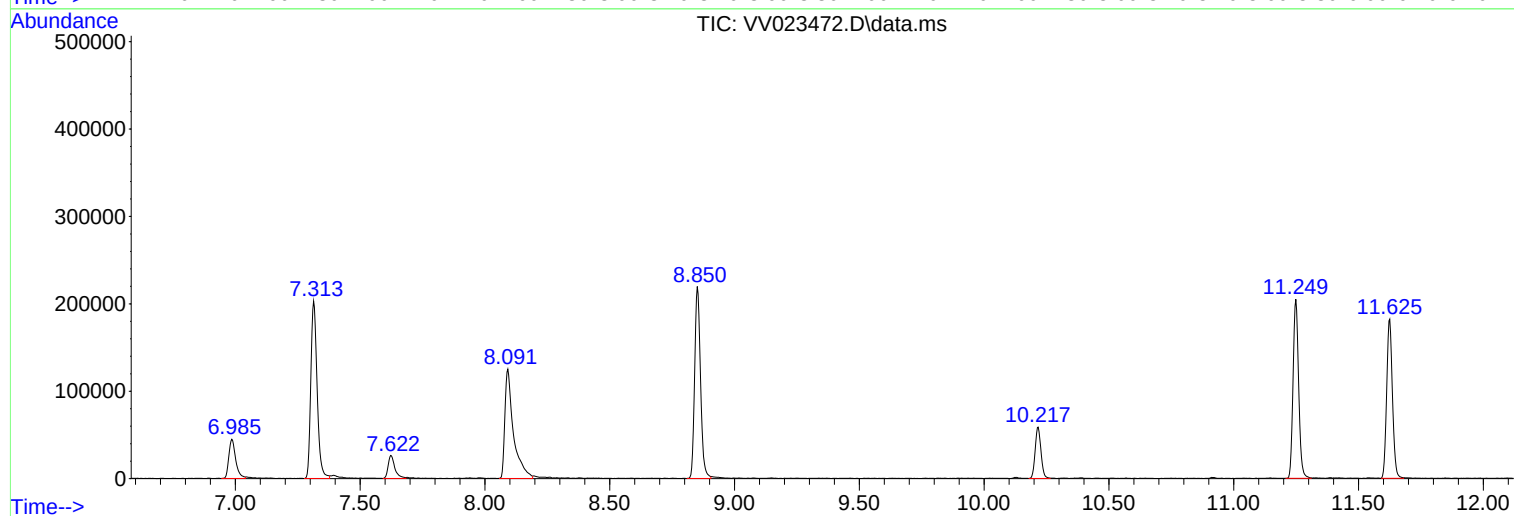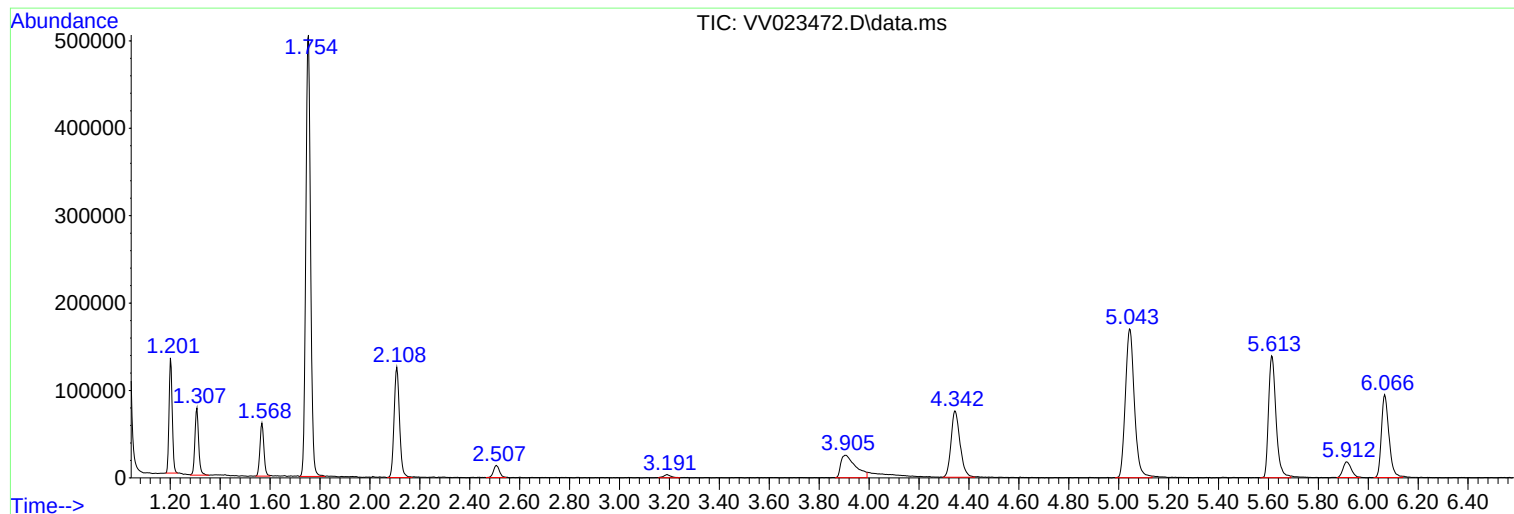

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023472.D
Acq On : 15 Nov 2021 11:09
Operator : SY/MD
Sample : M4616-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X7DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.97 ug/L	114370	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Cyanogen chloride	61	CClN	000506-77-4	4
4			Trifluoroguanidine	113	CH2F3N3	037950-72-4	4
5			Cyanogen chloride	61	CClN	000506-77-4	4

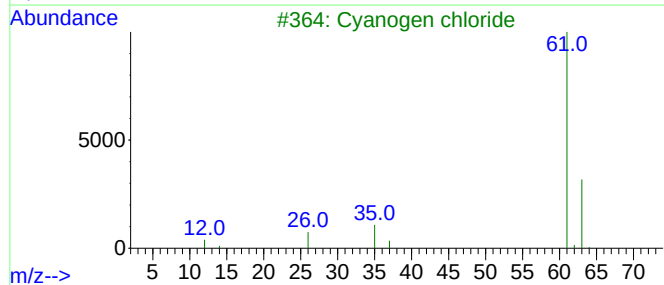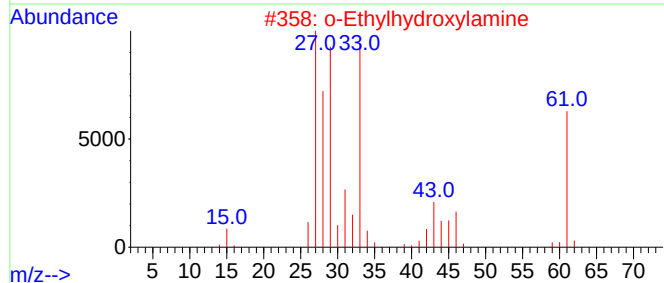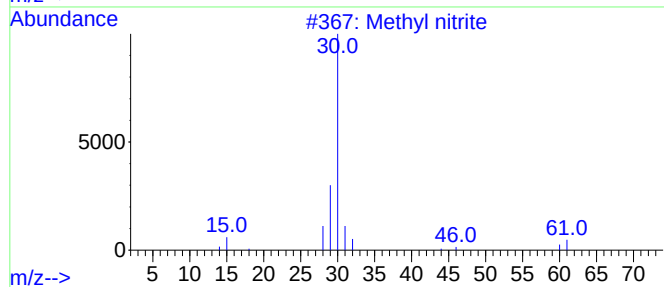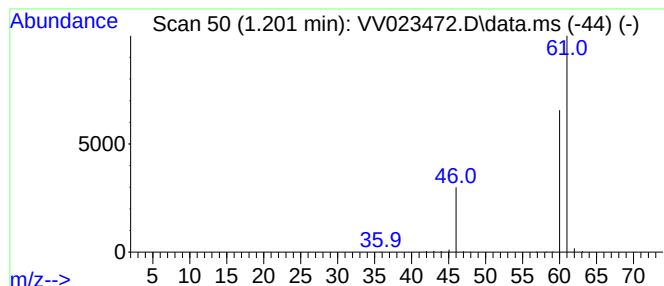

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023472.D
Acq On : 15 Nov 2021 11:09
Operator : SY/MD
Sample : M4616-04DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1X7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	2.0	ug/L	114370	1	5.616	289822	5.0