

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023479.D
 Acq On : 15 Nov 2021 13:55
 Operator : SY/MD
 Sample : M4616-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	40	rVB	13225	13001	1.17%	0.265%
2	1.201	45	50	58	rVV	38609	34801	3.12%	0.710%
3	1.307	76	83	94	rVB	74359	76081	6.82%	1.551%
4	1.568	157	164	180	rVB	60405	67866	6.08%	1.384%
5	2.111	320	333	346	rBV	117711	175324	15.71%	3.575%
6	3.902	877	890	921	rBV3	42307	151087	13.54%	3.081%
7	4.349	1013	1029	1055	rBV2	77415	204082	18.29%	4.162%
8	5.050	1230	1247	1277	rBV2	173334	435632	39.04%	8.884%
9	5.619	1409	1424	1444	rBV	138680	280991	25.18%	5.730%
10	5.915	1502	1516	1549	rBV	565770	1115722	100.00%	22.753%
11	6.069	1552	1564	1587	rVV	98209	201844	18.09%	4.116%
12	6.989	1838	1850	1877	rBV	48596	90697	8.13%	1.850%
13	7.317	1941	1952	1973	rBV	211311	369021	33.07%	7.525%
14	7.625	2038	2048	2071	rBV	28327	51738	4.64%	1.055%
15	7.976	2145	2157	2174	rVB	141183	241619	21.66%	4.927%
16	8.092	2183	2193	2224	rBV2	147728	309459	27.74%	6.311%
17	8.854	2418	2430	2454	rBV	219114	357780	32.07%	7.296%
18	10.217	2842	2854	2868	rBV2	59380	94698	8.49%	1.931%
19	11.249	3165	3175	3196	rBV	196934	307768	27.58%	6.276%
20	11.532	3254	3263	3278	rBV	13731	24104	2.16%	0.492%
21	11.625	3280	3292	3311	rVV	190561	300417	26.93%	6.126%




Sum of corrected areas: 4903732

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023479.D
Acq On : 15 Nov 2021 13:55
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

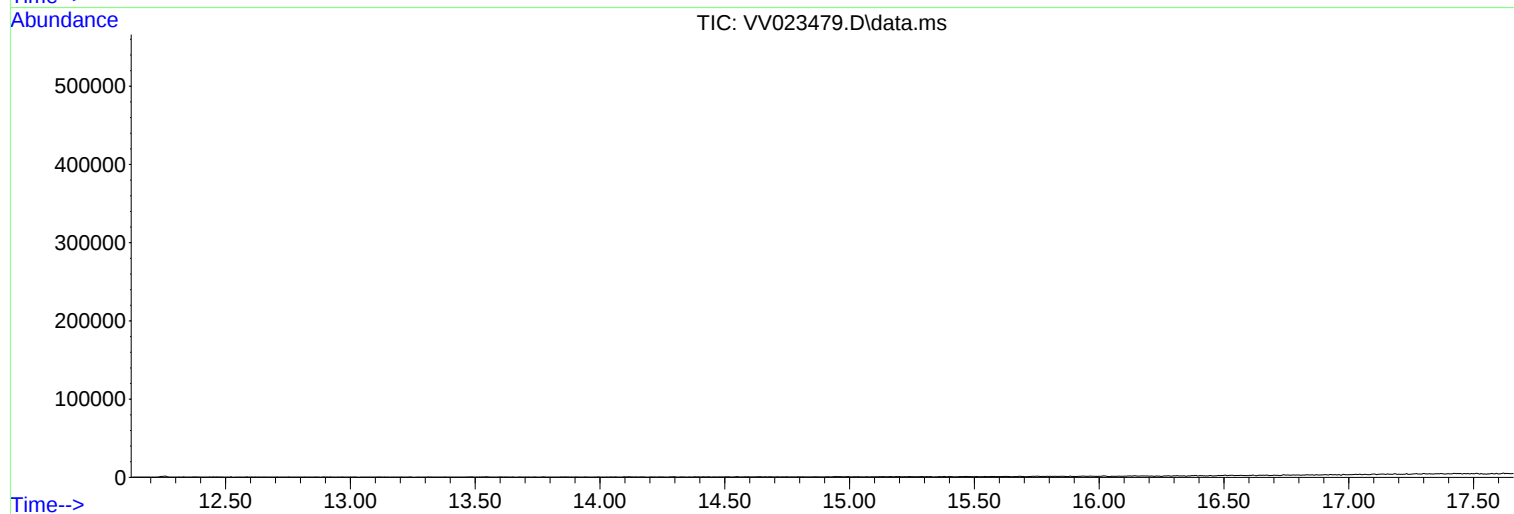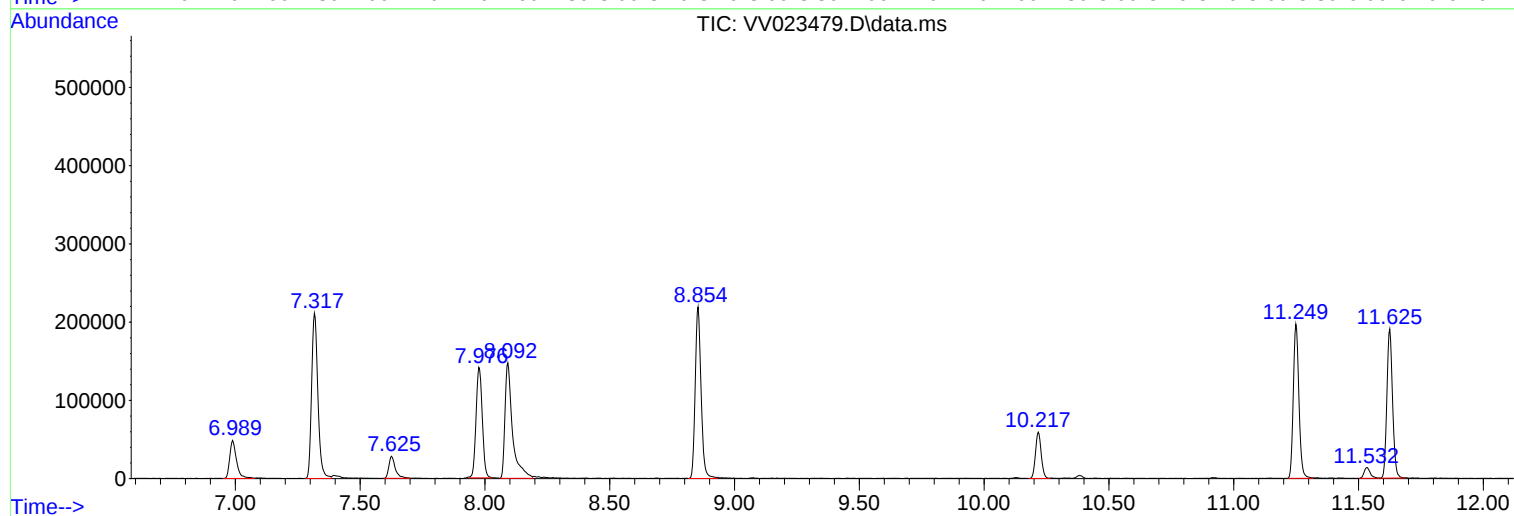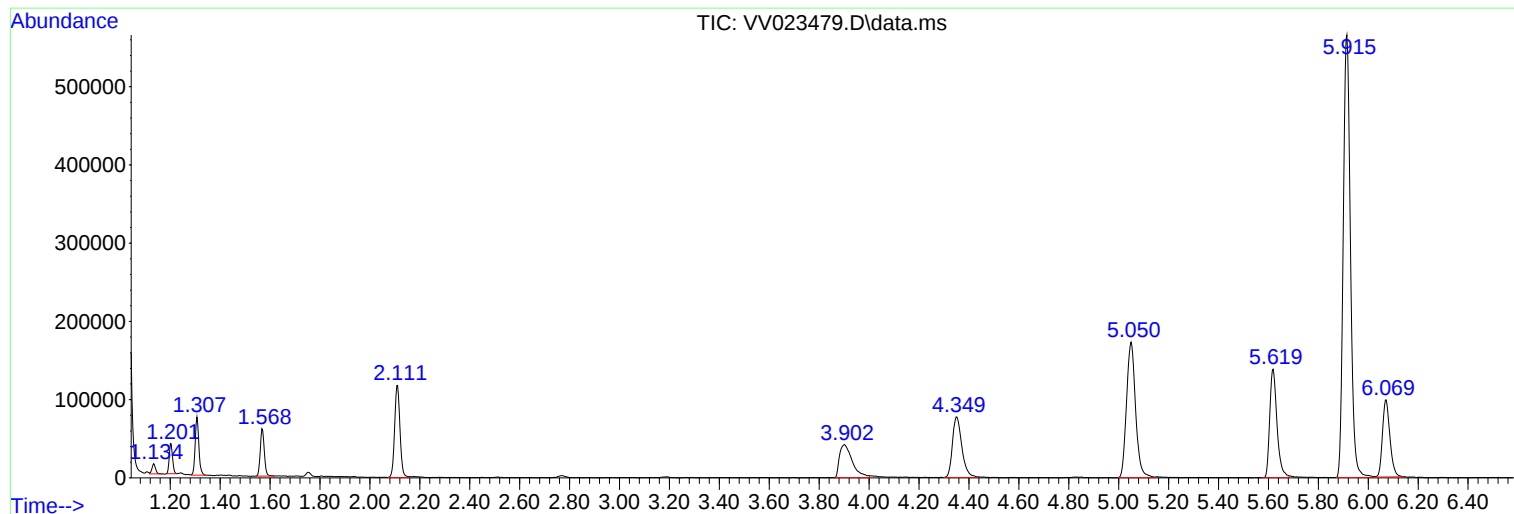

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023479.D
Acq On : 15 Nov 2021 13:55
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023479.D
Acq On : 15 Nov 2021 13:55
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc