

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023485.D
 Acq On : 15 Nov 2021 16:19
 Operator : SY/MD
 Sample : M4616-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	38	rVB	12014	12522	1.91%	0.295%
2	1.307	76	83	95	rVB	64079	65290	9.96%	1.536%
3	1.568	156	164	175	rBV	52948	59886	9.13%	1.409%
4	1.754	214	222	230	rBV2	7792	10096	1.54%	0.237%
5	2.108	319	332	349	rBV	105937	153720	23.44%	3.616%
6	3.912	881	893	918	rBV	29389	110192	16.80%	2.592%
7	4.352	1013	1030	1057	rBV2	70999	182348	27.81%	4.289%
8	5.050	1232	1247	1279	rBV3	154205	387307	59.06%	9.111%
9	5.619	1412	1424	1449	rBV	149118	309231	47.16%	7.274%
10	5.915	1500	1516	1549	rBV	327618	655757	100.00%	15.426%
11	6.069	1553	1564	1598	rVB	88604	186836	28.49%	4.395%
12	6.989	1841	1850	1868	rBV	41403	78964	12.04%	1.858%
13	7.317	1941	1952	1970	rBV	185255	326020	49.72%	7.669%
14	7.625	2038	2048	2063	rBV	25047	45274	6.90%	1.065%
15	7.976	2140	2157	2177	rBV2	151687	257225	39.23%	6.051%
16	8.095	2184	2194	2224	rBV2	129056	287618	43.86%	6.766%
17	8.853	2419	2430	2451	rBV	235398	384383	58.62%	9.042%
18	10.217	2844	2854	2871	rBV2	54886	87867	13.40%	2.067%
19	11.249	3164	3175	3197	rBV	219581	339539	51.78%	7.987%
20	11.532	3253	3263	3278	rBV2	18615	31715	4.84%	0.746%
21	11.625	3281	3292	3307	rBV	176609	279299	42.59%	6.570%




Sum of corrected areas: 4251089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023485.D
Acq On : 15 Nov 2021 16:19
Operator : SY/MD
Sample : M4616-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

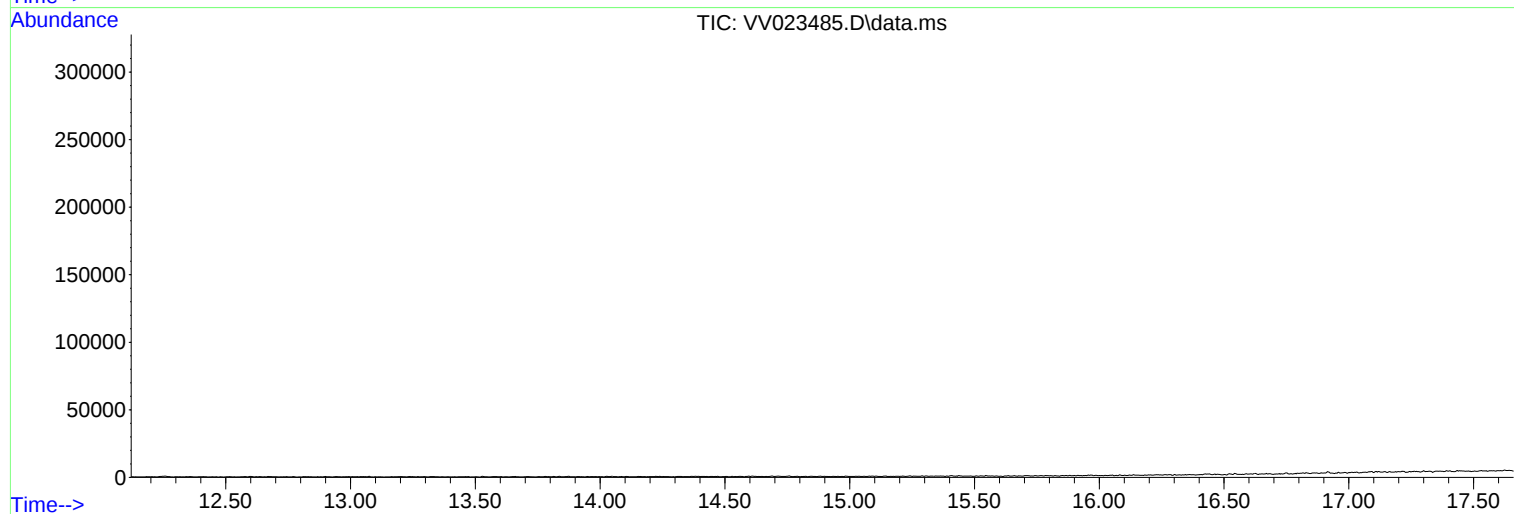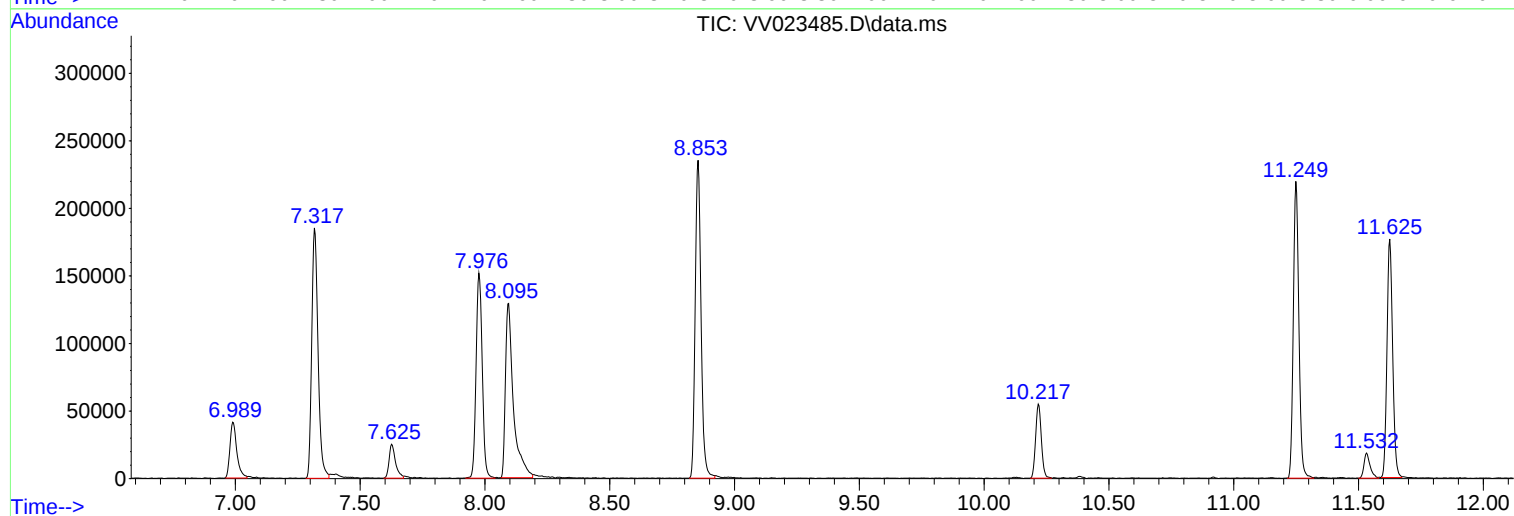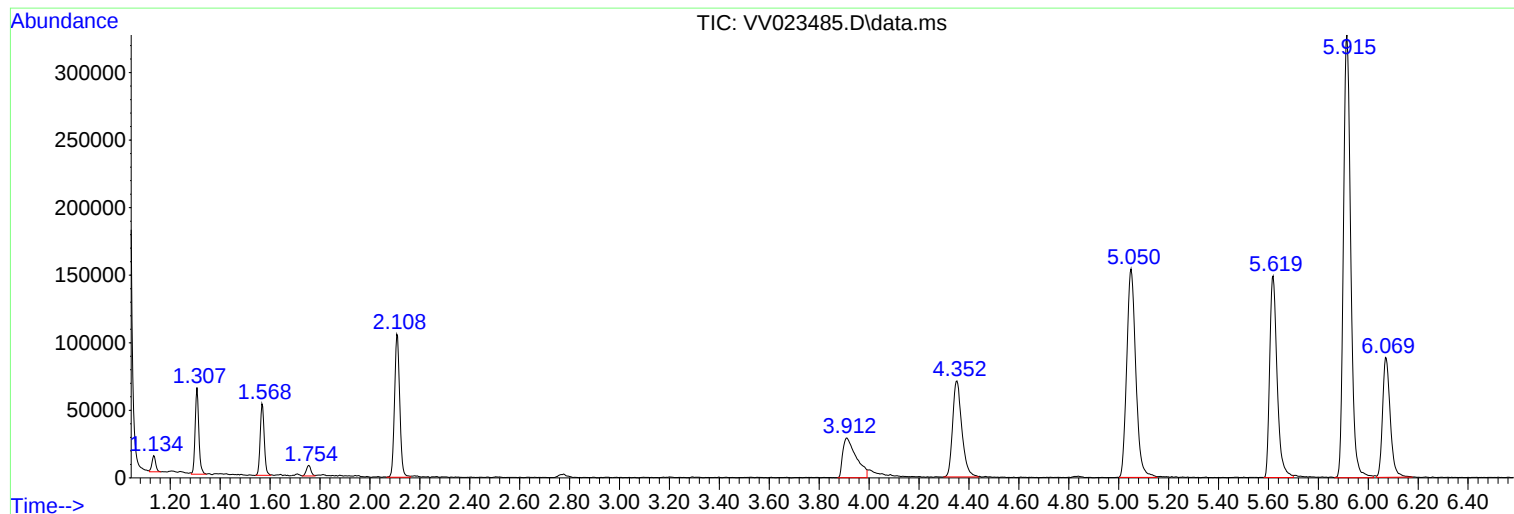

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023485.D
Acq On : 15 Nov 2021 16:19
Operator : SY/MD
Sample : M4616-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023485.D
Acq On : 15 Nov 2021 16:19
Operator : SY/MD
Sample : M4616-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc