

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023487.D
 Acq On : 15 Nov 2021 17:06
 Operator : SY/MD
 Sample : M4616-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Z0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	62	rBV	9242	9186	2.31%	0.247%
2	1.307	76	83	98	rVB	63059	66696	16.80%	1.791%
3	1.568	157	164	177	rBV	53233	60161	15.15%	1.616%
4	2.108	322	332	352	rBV	102432	152631	38.44%	4.099%
5	3.889	877	886	918	rBV	35388	118983	29.97%	3.195%
6	4.352	1014	1030	1062	rBV	73649	182903	46.06%	4.912%
7	5.050	1231	1247	1274	rBV2	156787	392800	98.93%	10.548%
8	5.619	1412	1424	1451	rBV	152930	315585	79.48%	8.474%
9	5.915	1503	1516	1545	rBV2	130096	266478	67.11%	7.156%
10	6.069	1550	1564	1586	rBV2	88942	185701	46.77%	4.987%
11	6.989	1840	1850	1872	rBV	42338	82018	20.66%	2.202%
12	7.317	1938	1952	1973	rBV	185378	328940	82.84%	8.833%
13	7.394	1973	1976	1992	rVB6	3175	5744	1.45%	0.154%
14	7.625	2039	2048	2067	rBV	25389	45906	11.56%	1.233%
15	7.976	2147	2157	2175	rVB2	51973	90589	22.81%	2.433%
16	8.092	2182	2193	2228	rBV2	135402	296793	74.75%	7.970%
17	8.854	2419	2430	2452	rBV	242943	397065	100.00%	10.662%
18	10.217	2842	2854	2868	rBV	54919	87048	21.92%	2.338%
19	10.387	2898	2907	2918	rVB2	3100	4815	1.21%	0.129%
20	11.249	3163	3175	3199	rBV	217943	344783	86.83%	9.259%
21	11.535	3256	3264	3276	rBV3	5922	10627	2.68%	0.285%
22	11.625	3281	3292	3308	rBV	177705	278500	70.14%	7.479%


Sum of corrected areas: 3723952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023487.D
Acq On : 15 Nov 2021 17:06
Operator : SY/MD
Sample : M4616-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

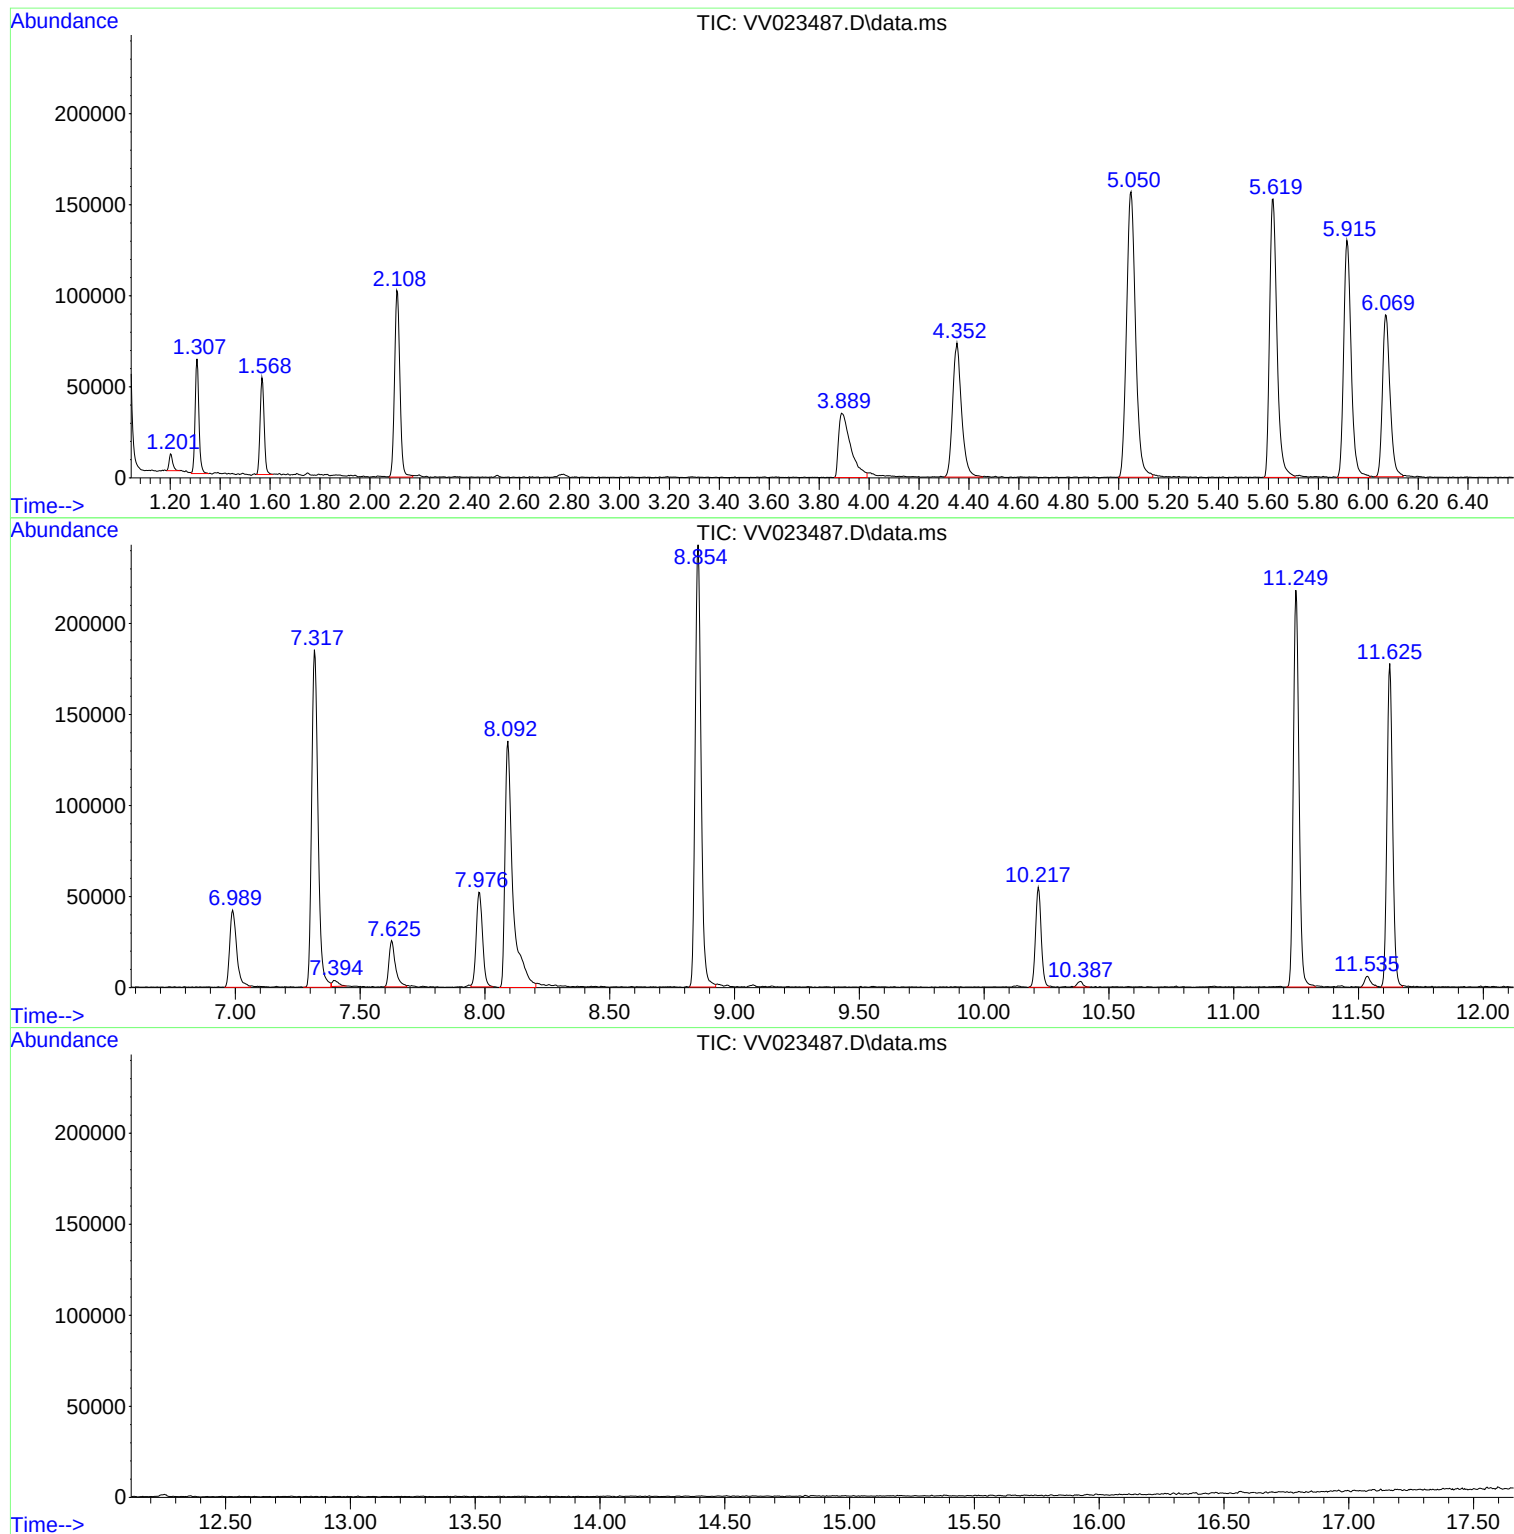

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023487.D
Acq On : 15 Nov 2021 17:06
Operator : SY/MD
Sample : M4616-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023487.D
Acq On : 15 Nov 2021 17:06
Operator : SY/MD
Sample : M4616-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc