

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023489.D
 Acq On : 15 Nov 2021 17:54
 Operator : SY/MD
 Sample : M4617-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG223

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	61	rVB	22709	20282	5.01%	0.559%
2	1.307	76	83	96	rVB	64139	67131	16.58%	1.850%
3	1.568	156	164	178	rBV	54776	62489	15.43%	1.722%
4	1.709	200	208	214	rBV	16475	19357	4.78%	0.533%
5	1.754	214	222	230	rVV	22178	27909	6.89%	0.769%
6	2.111	320	333	350	rBV3	125117	196477	48.53%	5.415%
7	2.770	526	538	553	rBV2	9535	21185	5.23%	0.584%
8	3.195	655	670	694	rBV3	27951	59834	14.78%	1.649%
9	3.896	878	888	925	rBV	36659	124322	30.71%	3.426%
10	4.352	1010	1030	1063	rBV2	76148	214688	53.03%	5.917%
11	4.606	1097	1109	1111	rBV3	6198	8500	2.10%	0.234%
12	5.050	1227	1247	1273	rBV4	160409	404858	100.00%	11.158%
13	5.619	1412	1424	1452	rBV	134954	276395	68.27%	7.618%
14	5.918	1501	1517	1544	rBV4	40949	87186	21.53%	2.403%
15	6.069	1552	1564	1588	rBV	91515	191693	47.35%	5.283%
16	6.989	1838	1850	1871	rBV	44041	83439	20.61%	2.300%
17	7.317	1941	1952	1973	rBV	191533	336815	83.19%	9.283%
18	7.625	2034	2048	2069	rBV2	26040	48708	12.03%	1.342%
19	7.976	2147	2157	2173	rVB3	21020	39046	9.64%	1.076%
20	8.092	2182	2193	2230	rBV2	136379	300488	74.22%	8.282%
21	8.854	2418	2430	2452	rBV	213952	349133	86.24%	9.622%
22	10.217	2842	2854	2874	rVB2	57493	92471	22.84%	2.549%
23	10.381	2897	2905	2913	rBV2	2838	4144	1.02%	0.114%
24	11.249	3164	3175	3195	rBV	196716	305322	75.41%	8.415%
25	11.538	3256	3265	3272	rBV6	3468	5302	1.31%	0.146%
26	11.625	3280	3292	3310	rBV	180086	281159	69.45%	7.749%




Sum of corrected areas: 3628333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023489.D
Acq On : 15 Nov 2021 17:54
Operator : SY/MD
Sample : M4617-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

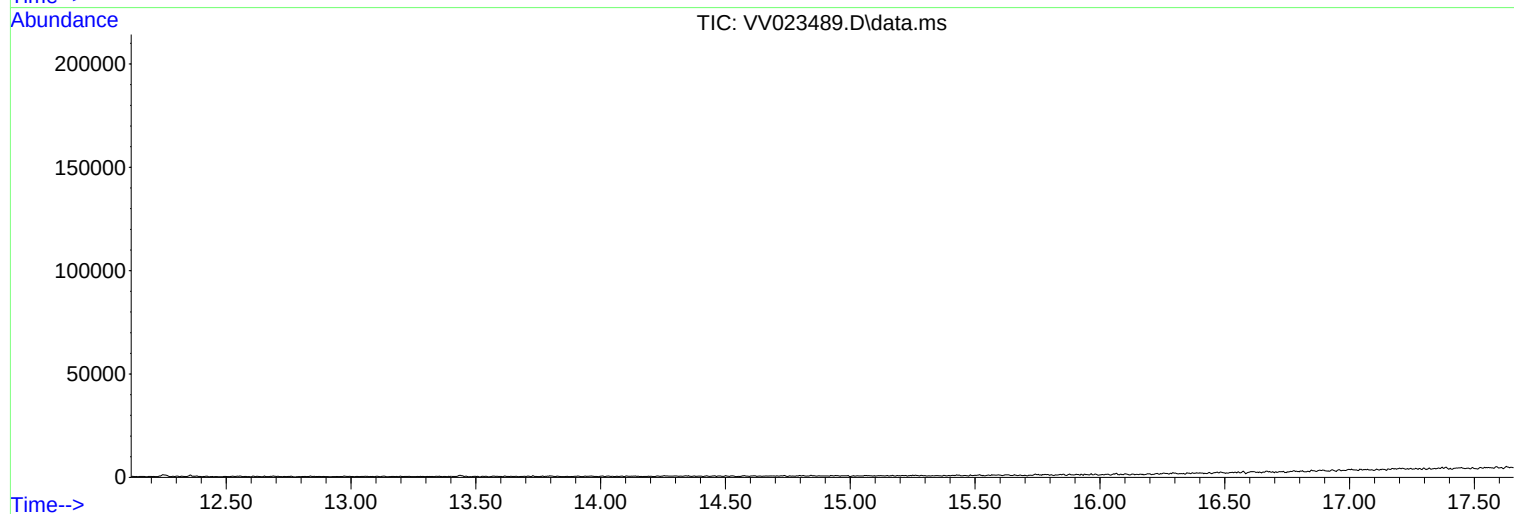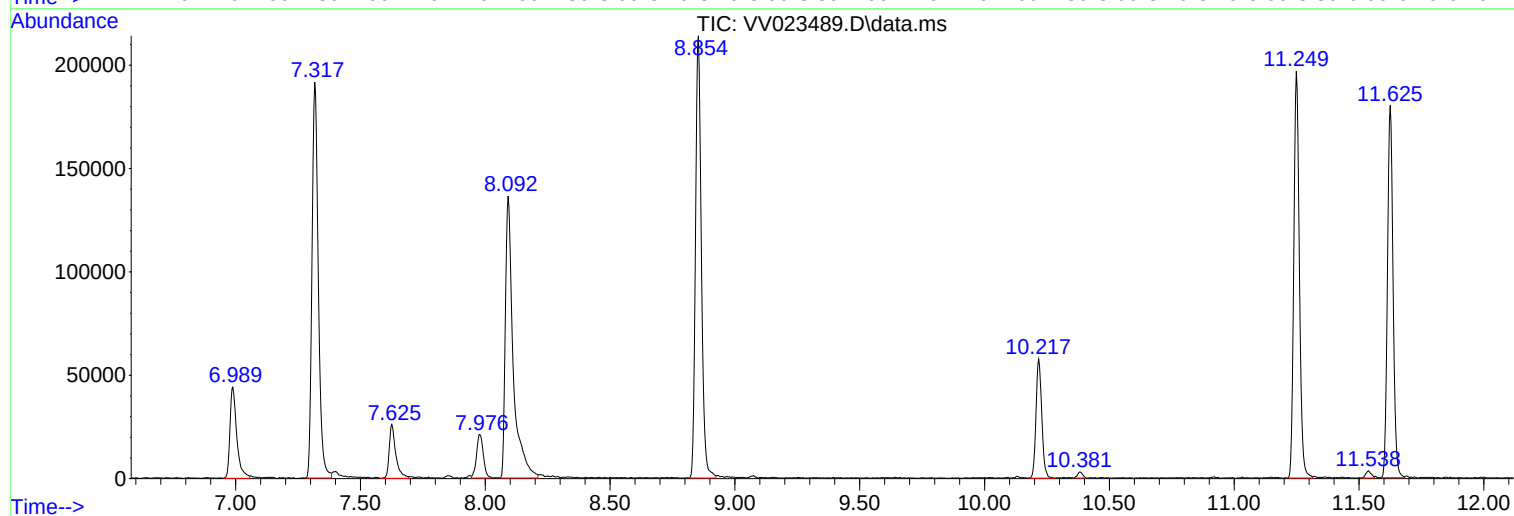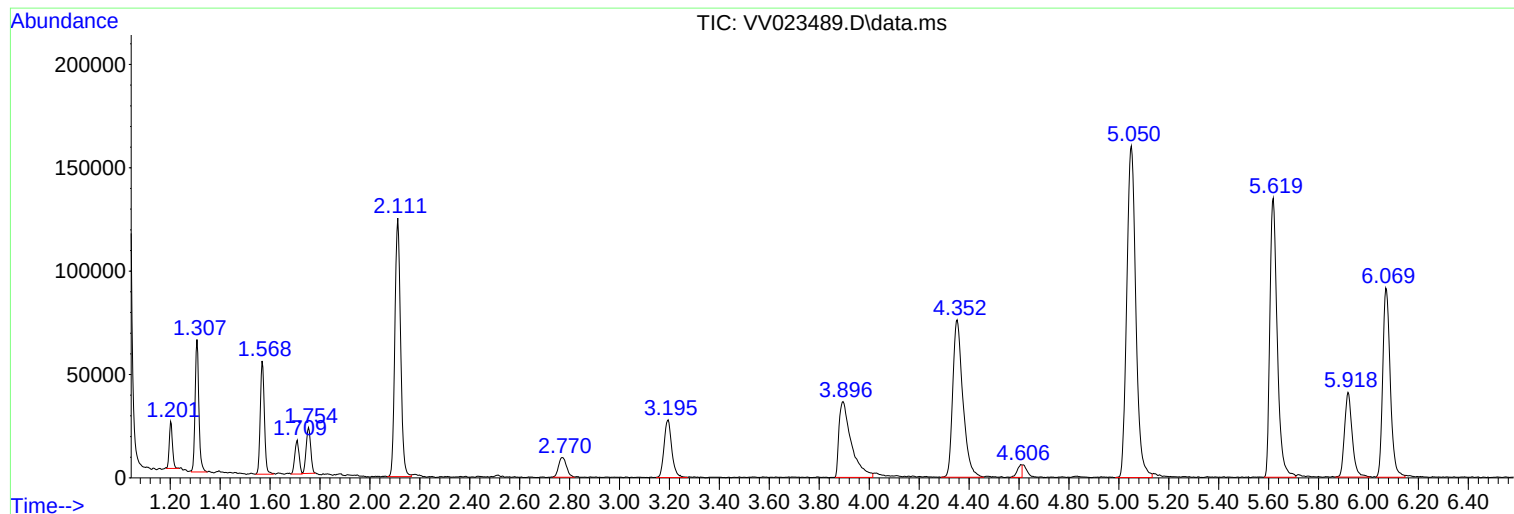

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023489.D
Acq On : 15 Nov 2021 17:54
Operator : SY/MD
Sample : M4617-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023489.D
Acq On : 15 Nov 2021 17:54
Operator : SY/MD
Sample : M4617-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc