

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023490.D
 Acq On : 15 Nov 2021 18:18
 Operator : SY/MD
 Sample : M4617-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG224

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	46	50	60	rVB2	5509	5440	1.37%	0.160%
2	1.307	76	83	98	rVB	63892	67019	16.94%	1.976%
3	1.568	155	164	176	rBV	50911	59456	15.03%	1.753%
4	2.108	321	332	347	rBV	102874	148518	37.53%	4.380%
5	2.773	527	539	551	rBV4	6352	14231	3.60%	0.420%
6	3.899	880	889	923	rBV2	28513	111981	28.30%	3.302%
7	4.355	1012	1031	1057	rBV2	69112	183039	46.26%	5.398%
8	5.050	1230	1247	1289	rBV2	158853	395699	100.00%	11.669%
9	5.619	1411	1424	1449	rBV	133787	277349	70.09%	8.179%
10	5.918	1505	1517	1533	rBV9	10479	24254	6.13%	0.715%
11	6.072	1552	1565	1588	rBV	89863	185465	46.87%	5.469%
12	6.989	1840	1850	1872	rBV	42783	79035	19.97%	2.331%
13	7.317	1941	1952	1973	rBV	183701	323554	81.77%	9.541%
14	7.625	2038	2048	2071	rBV	24100	45111	11.40%	1.330%
15	7.976	2146	2157	2180	rVB	88720	152267	38.48%	4.490%
16	8.092	2183	2193	2229	rBV3	132818	296008	74.81%	8.729%
17	8.854	2418	2430	2454	rBV	209573	347627	87.85%	10.251%
18	10.217	2843	2854	2871	rBV3	55957	87062	22.00%	2.567%
19	11.249	3162	3175	3196	rBV	196401	305364	77.17%	9.005%
20	11.538	3256	3265	3274	rBV3	4931	8331	2.11%	0.246%
21	11.625	3279	3292	3310	rVV	176470	274341	69.33%	8.090%




Sum of corrected areas: 3391151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023490.D
Acq On : 15 Nov 2021 18:18
Operator : SY/MD
Sample : M4617-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

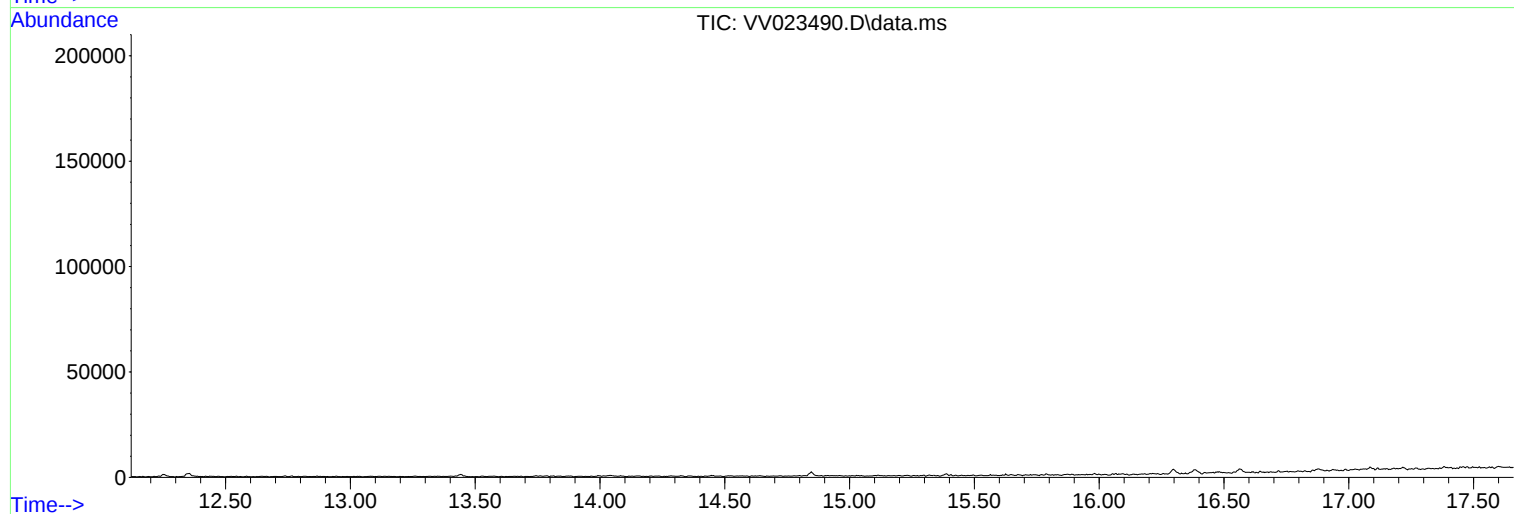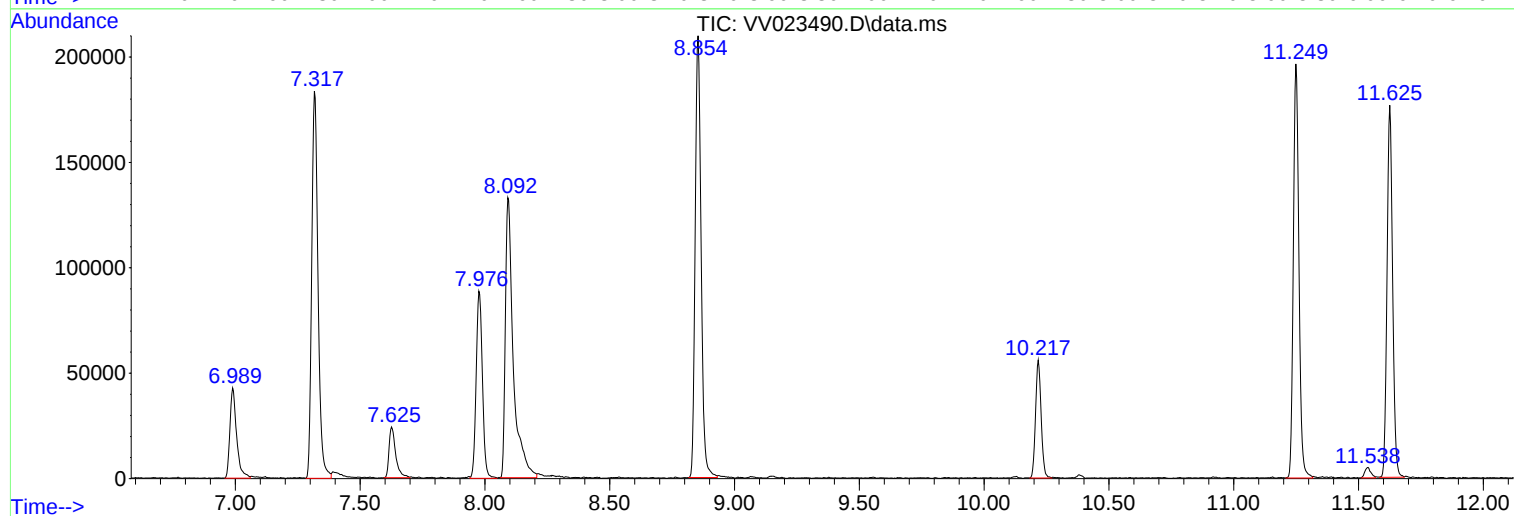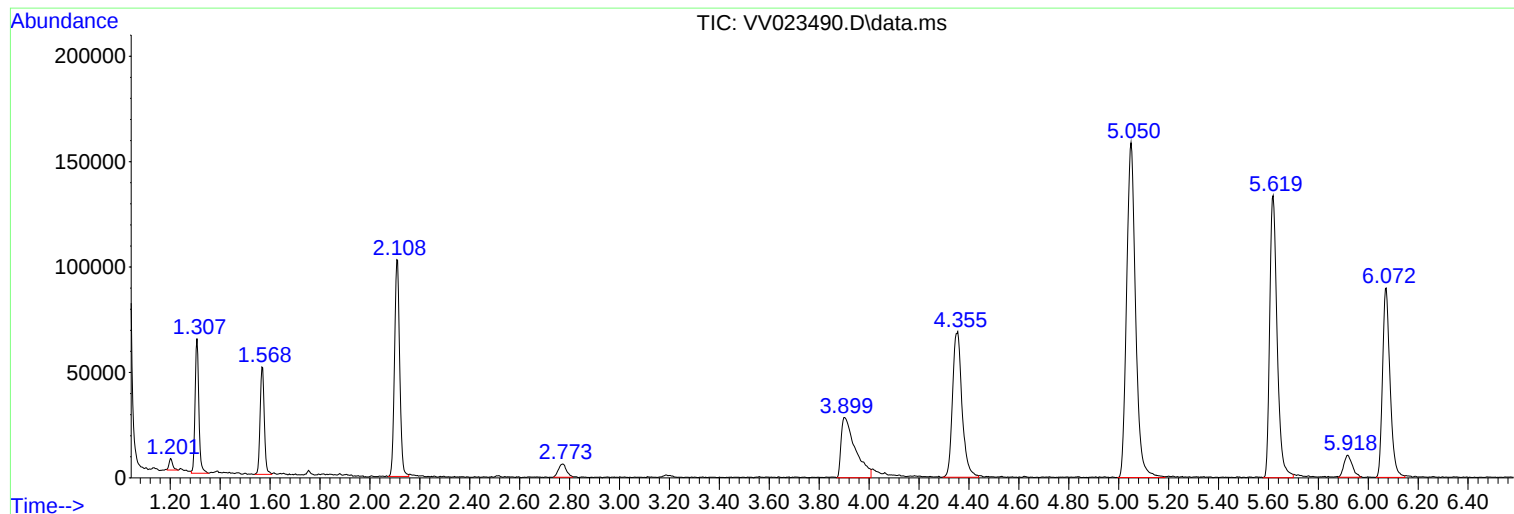

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023490.D
Acq On : 15 Nov 2021 18:18
Operator : SY/MD
Sample : M4617-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023490.D
Acq On : 15 Nov 2021 18:18
Operator : SY/MD
Sample : M4617-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG224

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc