

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023514.D
 Acq On : 16 Nov 2021 03:54
 Operator : SY/MD
 Sample : M4694-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4652

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	61	rBV	25180	21531	1.03%	0.295%
2	1.311	76	84	106	rVB	1531510	1623018	77.91%	22.201%
3	1.571	157	165	174	rBV	55714	63016	3.02%	0.862%
4	1.635	179	185	196	rVB	16452	22335	1.07%	0.306%
5	2.111	322	333	350	rVB	109076	166230	7.98%	2.274%
6	2.581	468	479	493	rVB2	14376	25523	1.23%	0.349%
7	2.764	523	536	561	rBV2	112147	229261	11.00%	3.136%
8	3.912	875	893	937	rBV	830870	2083326	100.00%	28.497%
9	4.349	1009	1029	1055	rBV	74969	189573	9.10%	2.593%
10	5.050	1229	1247	1285	rBV2	170501	459866	22.07%	6.290%
11	5.619	1412	1424	1450	rBV	142533	296854	14.25%	4.061%
12	6.072	1550	1565	1593	rBV	95047	199401	9.57%	2.728%
13	6.989	1840	1850	1866	rBV2	44430	85309	4.09%	1.167%
14	7.317	1941	1952	1971	rBV	203072	354764	17.03%	4.853%
15	7.625	2038	2048	2065	rBV	25804	46547	2.23%	0.637%
16	8.092	2184	2193	2229	rBV2	159221	339652	16.30%	4.646%
17	8.854	2419	2430	2459	rBV	217971	360894	17.32%	4.937%
18	10.217	2840	2854	2867	rBV2	66066	105455	5.06%	1.443%
19	11.249	3164	3175	3202	rBV	210984	332811	15.97%	4.552%
20	11.625	3280	3292	3310	rBV	189986	305194	14.65%	4.175%




Sum of corrected areas: 7310560

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023514.D
Acq On : 16 Nov 2021 03:54
Operator : SY/MD
Sample : M4694-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

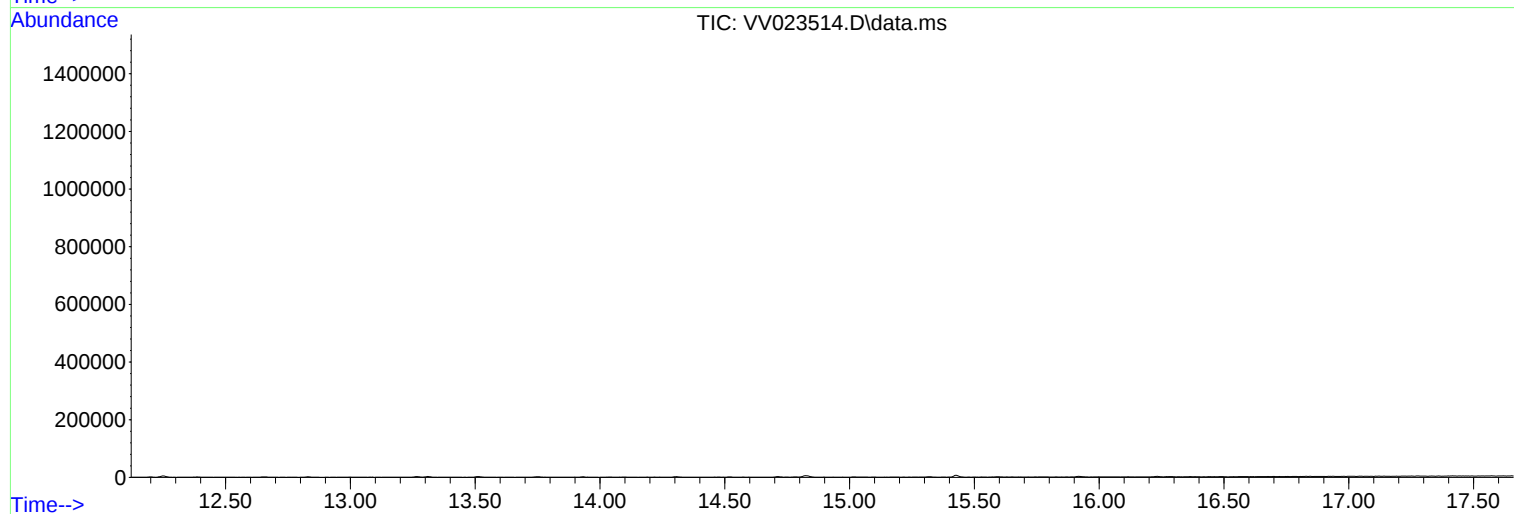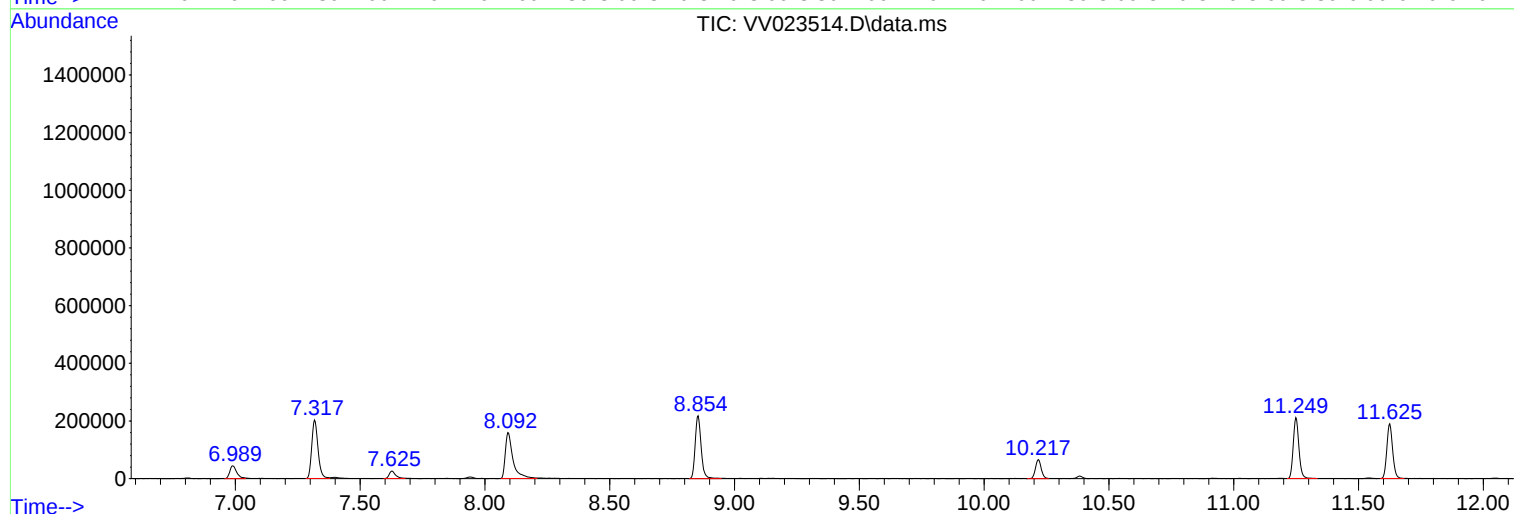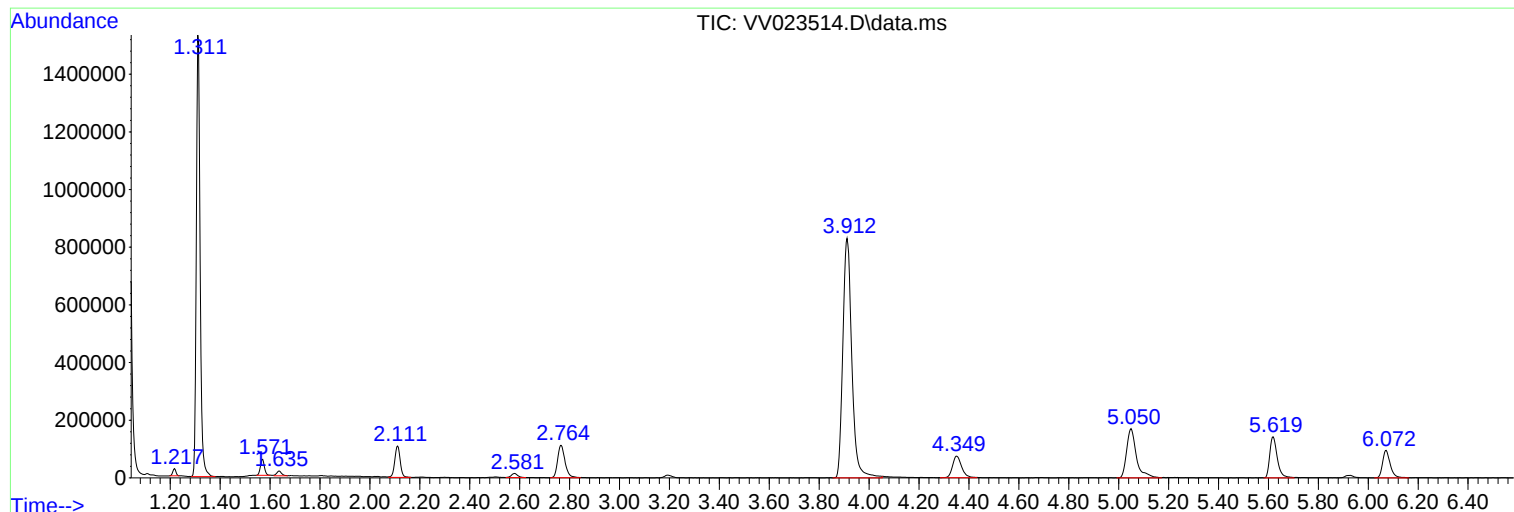

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023514.D
Acq On : 16 Nov 2021 03:54
Operator : SY/MD
Sample : M4694-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
Data File : VV023514.D
Acq On : 16 Nov 2021 03:54
Operator : SY/MD
Sample : M4694-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc