
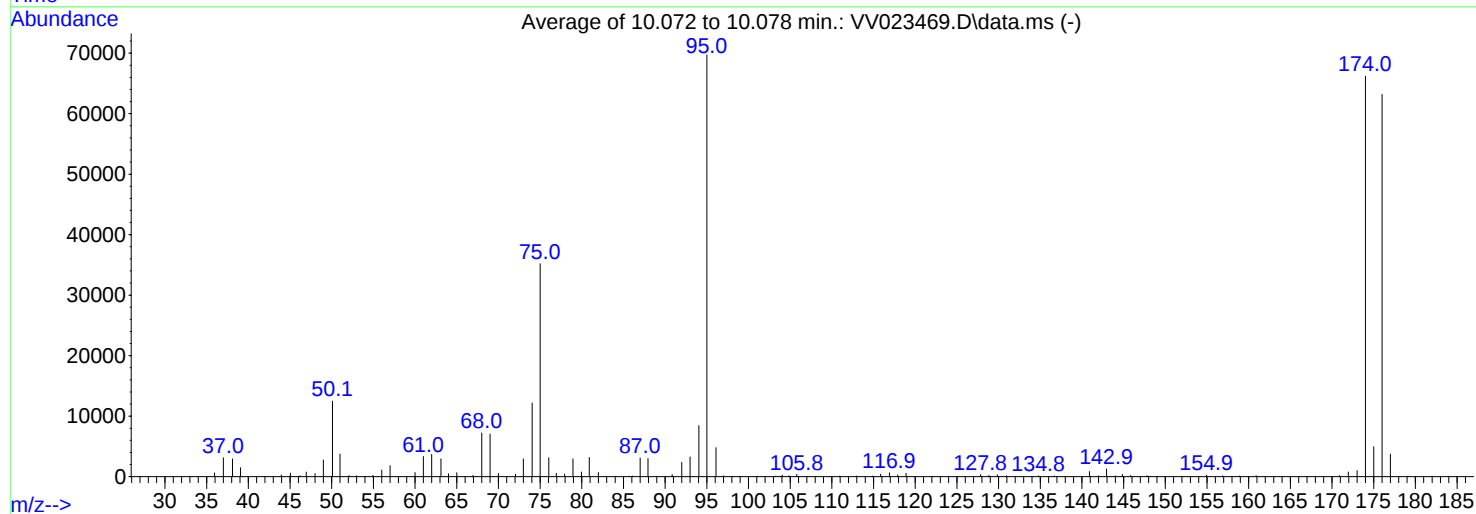


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111521\
 Data File : VV023469.D
 Acq On : 15 Nov 2021 09:08
 Operator : SY/MD
 Sample : BFB234
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB234

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 18 00:20:29 2021

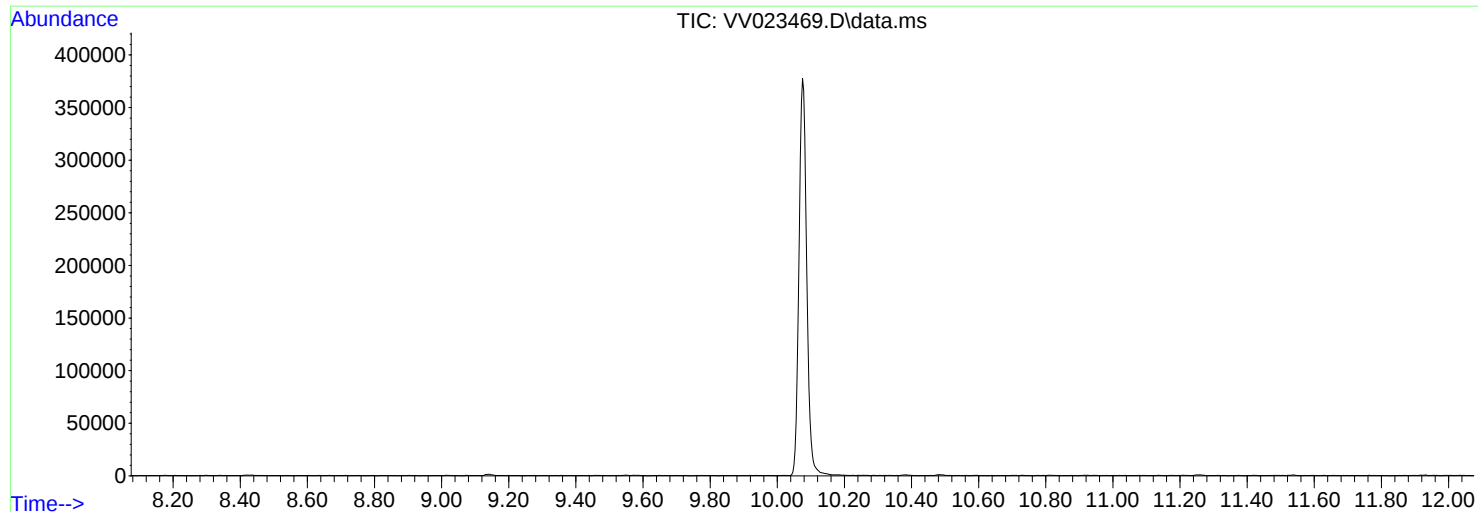

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	12487	PASS
75	95	30	80	50.5	35208	PASS
95	95	100	100	100.0	69725	PASS
96	95	5	9	6.9	4782	PASS
173	174	0.00	2	1.5	1013	PASS
174	95	50	120	94.9	66195	PASS
175	174	5	9	7.5	4959	PASS
176	174	95	105	95.4	63176	PASS
177	176	5	10	5.9	3706	PASS

m/z	Abundance
39.90	129.0
43.90	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.00	613.0
37.00	3222.0
38.10	2697.0
39.00	1408.0
40.00	153.0
44.00	508.0
45.00	526.0
46.20	140.0
47.00	853.0
48.00	491.0
49.00	2662.0
50.10	12350.0
51.00	3600.0
52.10	182.0
52.90	188.0
54.90	183.0
56.00	1048.0
57.00	1933.0
60.00	725.0
61.00	3369.0
62.00	3399.0
63.10	2963.0
64.00	554.0
65.00	676.0
66.90	250.0
68.00	7085.0
69.00	6921.0
70.00	468.0
72.10	406.0
73.00	2764.0
74.00	12048.0
75.00	34448.0
76.00	2987.0
76.90	528.0
77.90	355.0
78.90	2922.0
79.90	742.0
80.90	3111.0
82.00	670.0
87.00	3101.0
88.00	2919.0
90.80	347.0
92.00	2287.0
93.00	3081.0
94.10	7994.0
95.00	67760.0
96.10	4798.0
97.00	121.0
104.00	273.0
104.80	157.0
105.80	358.0
111.00	105.0
114.90	108.0
115.80	392.0
116.90	608.0
117.90	299.0
118.90	524.0
127.80	299.0
128.80	214.0
129.90	283.0
131.00	139.0
134.70	126.0
140.90	786.0
142.00	113.0
143.00	1319.0
144.00	122.0
144.80	386.0
145.90	174.0
147.80	198.0
155.00	228.0
156.80	124.0
158.90	110.0
160.90	138.0
170.90	207.0
172.00	765.0
173.00	913.0
174.00	63816.0
175.00	4757.0
176.00	60240.0
177.00	3694.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.90	603.0
37.00	3203.0
38.10	3026.0
39.00	1534.0
40.00	160.0
44.00	497.0
45.10	597.0
46.20	182.0
46.90	759.0
48.00	519.0
49.00	2861.0
50.10	12993.0
51.00	3858.0
52.10	197.0
53.00	169.0
55.00	201.0
56.00	1141.0
57.00	1872.0
60.00	694.0
61.00	3417.0
62.00	3788.0
63.10	3023.0
64.00	477.0
65.00	696.0
67.00	218.0
68.00	7451.0
69.00	7295.0
70.00	557.0
72.00	400.0
73.00	2986.0
74.10	12574.0
75.00	36328.0
76.00	3260.0
76.90	556.0
77.90	438.0
78.90	3096.0
80.00	775.0
80.90	3304.0
82.00	702.0
82.90	116.0
85.70	115.0
86.10	138.0
87.00	3229.0
87.90	3026.0
90.80	361.0
92.00	2431.0
93.00	3371.0
94.00	8652.0
95.00	71752.0
96.10	4944.0
97.00	150.0
103.20	116.0
104.10	281.0
104.80	183.0
105.80	381.0
110.90	120.0
113.00	146.0
114.90	116.0
115.90	417.0
116.90	653.0
117.90	291.0
118.90	559.0
127.80	372.0
128.90	206.0
129.80	334.0
131.00	154.0
134.80	118.0
136.70	122.0
140.90	873.0
141.90	151.0
142.90	1315.0
144.00	134.0
144.90	374.0
145.80	190.0
147.80	150.0
148.10	140.0
155.00	232.0
156.80	151.0
158.90	112.0
160.90	164.0
170.90	170.0
172.00	775.0
173.00	1040.0
174.00	68304.0
175.00	5081.0
176.00	65248.0
177.00	3793.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.00	602.0
37.00	2969.0
38.10	3060.0
39.10	1502.0
40.00	182.0
44.00	482.0
45.10	600.0
46.20	162.0
47.00	684.0
48.00	484.0
49.00	2752.0
50.10	12118.0
51.00	3732.0
52.10	199.0
53.00	151.0
55.00	223.0
56.00	1072.0
57.00	1671.0
60.00	653.0
61.00	3225.0
62.00	3828.0
63.10	2816.0
64.00	441.0
65.00	654.0
67.00	204.0
68.00	7094.0
69.00	6862.0
70.00	574.0
72.00	388.0
73.00	3076.0
74.10	11866.0
75.00	34848.0
76.10	3139.0
77.00	566.0
78.00	482.0
79.00	2822.0
80.00	768.0
80.90	3105.0
82.00	725.0
82.90	107.0
85.70	119.0
86.10	150.0
87.00	2954.0
87.90	2997.0
90.90	345.0
92.00	2316.0
93.00	3281.0
94.00	8683.0
95.00	69664.0
96.10	4603.0
97.10	157.0
103.20	115.0
103.80	271.0
104.10	263.0
104.90	153.0
105.80	362.0
109.70	105.0
110.90	119.0
113.00	145.0
114.90	114.0
115.90	393.0
116.90	643.0
117.90	258.0
118.90	564.0
127.90	371.0
128.90	196.0
129.90	333.0
130.80	158.0
134.90	139.0
136.70	169.0
140.90	912.0
141.90	175.0
142.90	1189.0
144.00	129.0
144.90	355.0
145.80	198.0
147.80	112.0
148.20	140.0
154.90	240.0
156.90	145.0
158.90	102.0
160.90	150.0
170.90	136.0
171.90	810.0
173.00	1085.0
174.00	66464.0
175.00	5040.0
176.00	64040.0
177.00	3631.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234