

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV028978.D
 Acq On : 15 Nov 2022 10:56
 Operator : SY/MD
 Sample : VV1115WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Quant Time: Nov 16 03:17:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 16 03:16:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	290836	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	272930	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	128983	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	64416	3.633	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.568	69	67271	4.316	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.400%
11) 1,1-Dichloroethene-d2	2.105	63	98222	3.040	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.800%
20) 2-Butanone-d5	3.902	46	115504	38.916	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.840%
24) Chloroform-d	4.339	84	181317	4.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.024	65	82232	5.021	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.400%
32) Benzene-d6	5.043	84	363451	4.461	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	6.063	67	110230	4.846	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.310	98	319669	4.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.619	79	29497	3.976	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.600%
46) 2-Hexanone-d5	8.088	63	159859	50.478	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.960%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	76643	4.859	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.615	152	119863	5.194	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	21009	0.923	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028978.D
Acq On : 15 Nov 2022 10:56
Operator : SY/MD
Sample : VV1115WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Time: Nov 16 03:17:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 16 03:16:14 2022
Response via : Initial Calibration

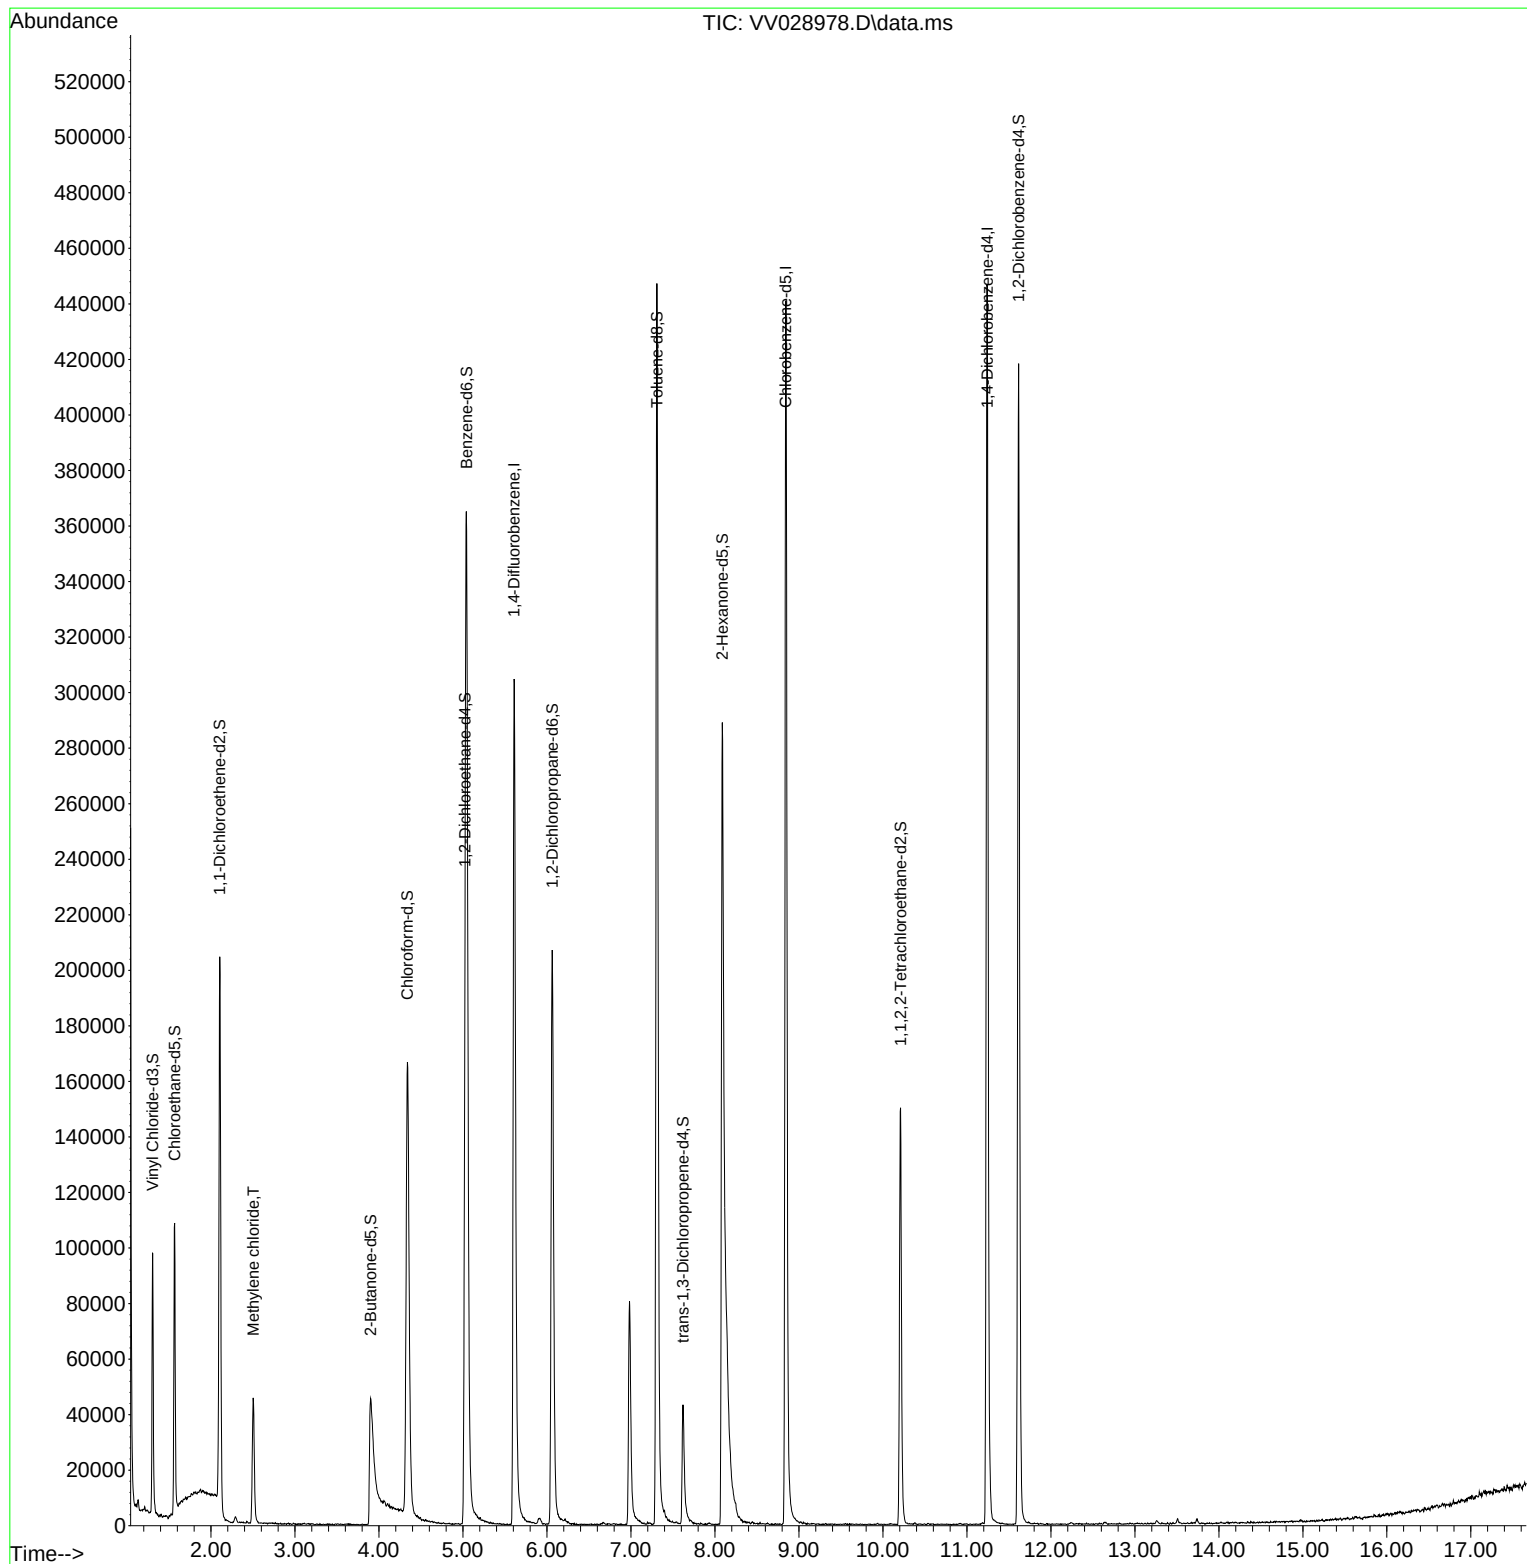

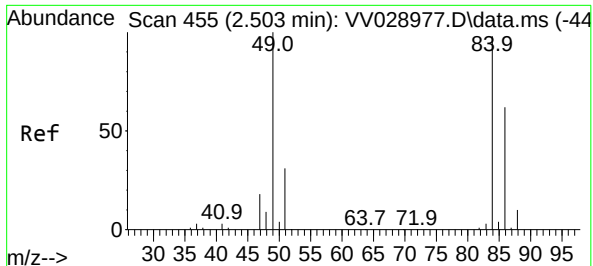

#16
Methylene chloride
Concen: 0.923 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV028978.D
Acq: 15 Nov 2022 10:56

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Tgt Ion: 84 Resp: 21009
Ion Ratio Lower Upper
84 100
86 65.4 45.8 85.0
49 96.9 75.5 140.1

