

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111522\
 Data File : VW028979.D
 Acq On : 15 Nov 2022 11:17
 Operator : SY/MD
 Sample : N5602-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 16 03:17:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 16 03:16:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	276879	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	257013	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	121407	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	68706	4.070	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.400%	
7) Chloroethane-d5	1.568	69	68159	4.593	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.108	63	97309	3.163	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.905	46	110164	38.988	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	77.980%	
24) Chloroform-d	4.349	84	180935	5.221	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	5.034	65	81401	5.220	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.050	84	361936	4.718	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.069	67	107932	5.038	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.800%	
41) Toluene-d8	7.313	98	320422	4.640	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.625	79	30161	4.317	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.400%	
46) 2-Hexanone-d5	8.092	63	163766	54.914	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.820%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	81369	5.479	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	109.600%	
66) 1,2-Dichlorobenzene-d4	11.616	152	114313	5.263	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.200%	
Target Compounds						
16) Methylene chloride	2.510	84	18928	0.873	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028979.D
Acq On : 15 Nov 2022 11:17
Operator : SY/MD
Sample : N5602-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 16 03:17:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 16 03:16:14 2022
Response via : Initial Calibration

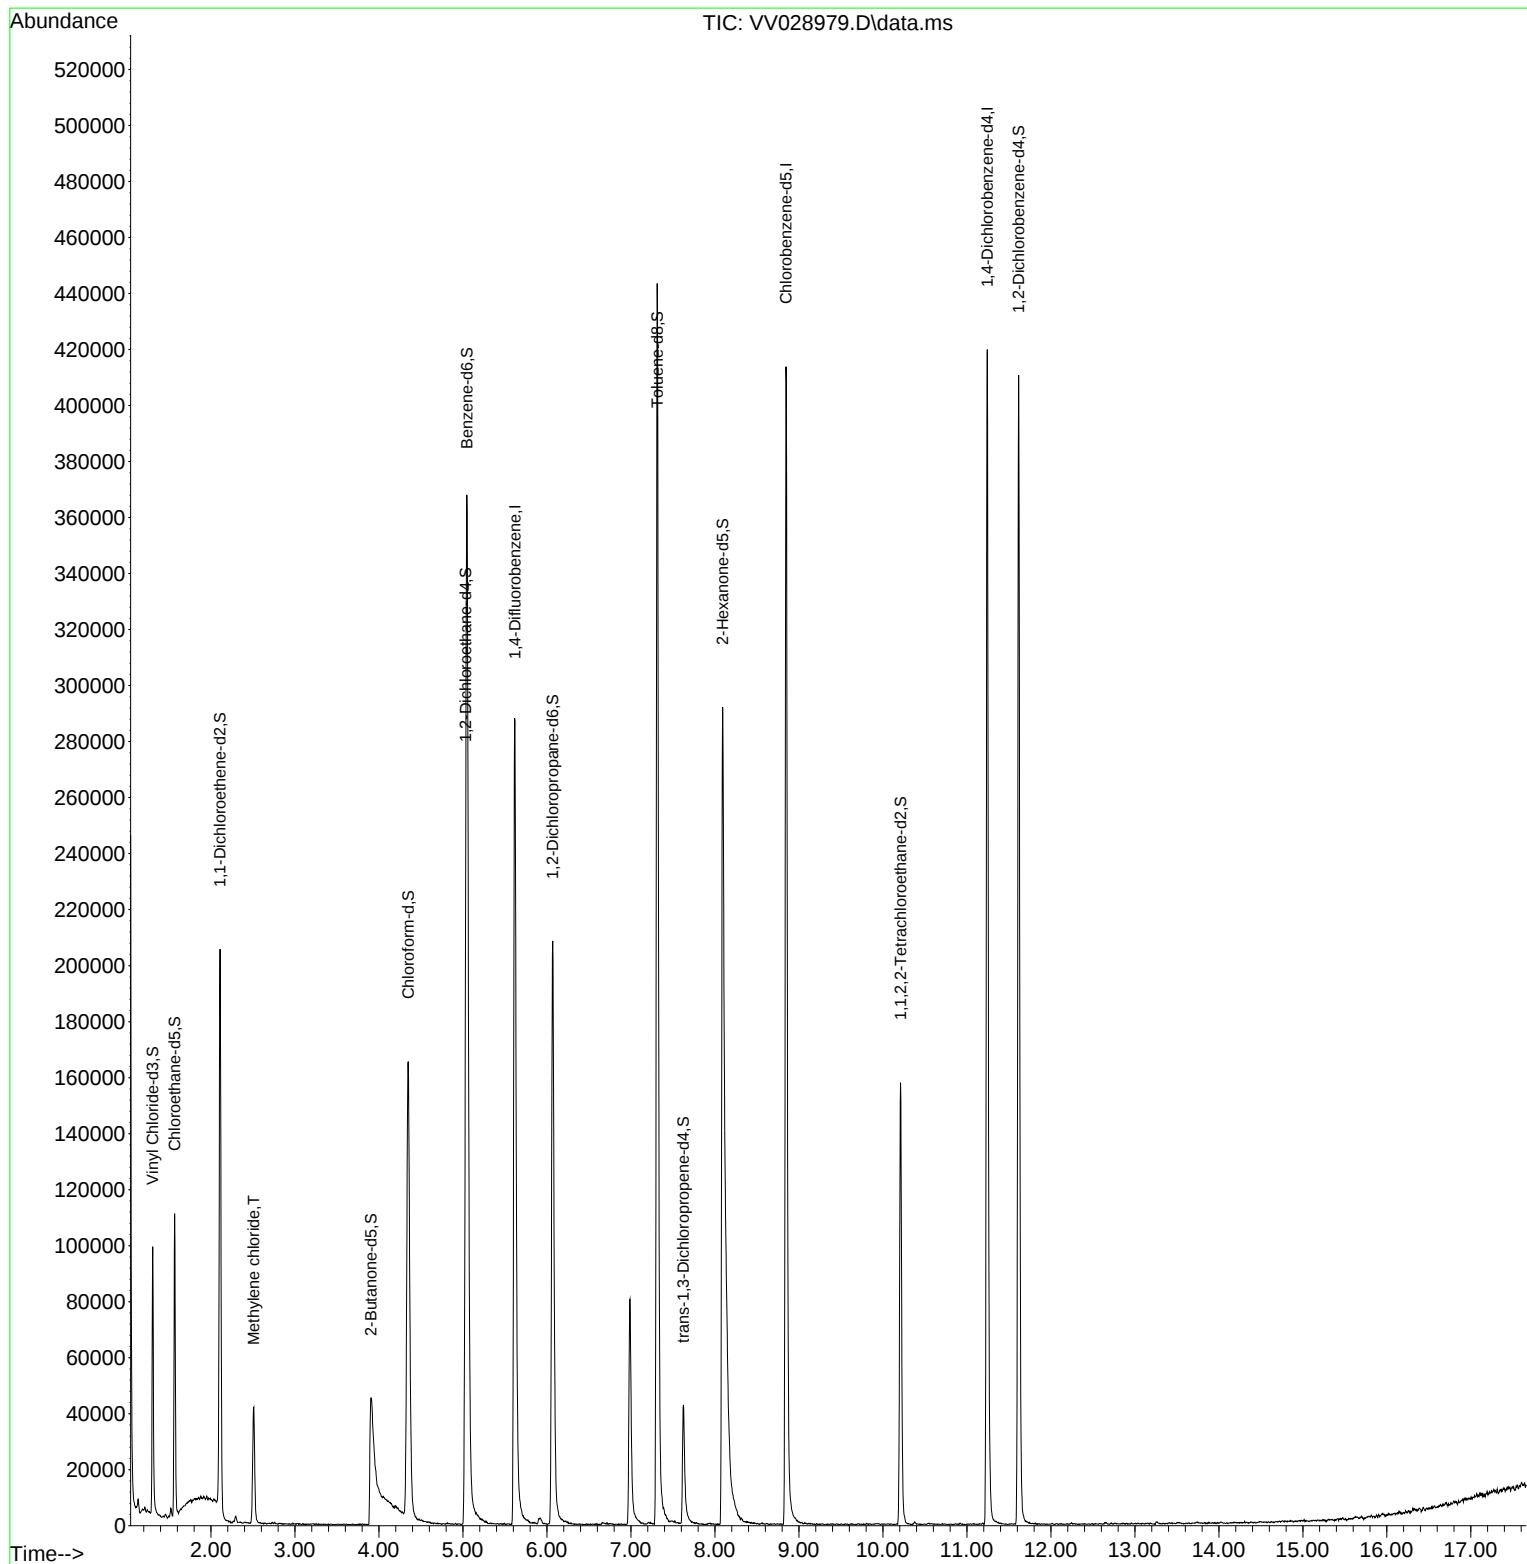

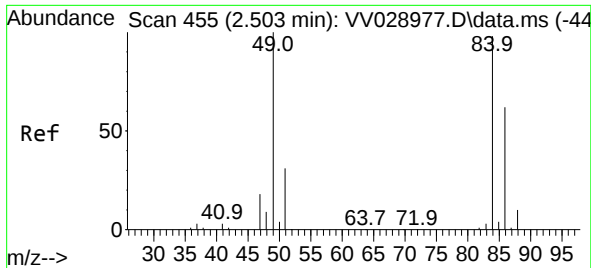

#16
Methylene chloride
Concen: 0.873 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV028979.D
Acq: 15 Nov 2022 11:17

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 18928
Ion Ratio Lower Upper
84 100
86 65.3 45.8 85.0
49 108.4 75.5 140.1

