

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111522\
 Data File : VW028998.D
 Acq On : 15 Nov 2022 18:58
 Operator : SY/MD
 Sample : N5593-02DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AD0DL

Quant Time: Nov 16 03:21:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 16 03:16:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	271657	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	251775	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	116353	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	45276	2.734	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	54.600%	
7) Chloroethane-d5	1.568	69	51540	3.540	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	70.800%	
11) 1,1-Dichloroethene-d2	2.105	63	71637	2.374	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	47.400%#	
20) 2-Butanone-d5	3.905	46	117230	42.286	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.580%	
24) Chloroform-d	4.342	84	145927	4.292	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.800%	
26) 1,2-Dichloroethane-d4	5.031	65	70322	4.597	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.000%	
32) Benzene-d6	5.047	84	286734	3.815	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	76.400%	
36) 1,2-Dichloropropane-d6	6.066	67	87459	4.168	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	83.400%	
41) Toluene-d8	7.310	98	242954	3.591	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	71.800%	
43) trans-1,3-Dichloroprop...	7.622	79	24863	3.633	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	72.600%	
46) 2-Hexanone-d5	8.088	63	139621	47.791	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.580%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	69457	4.774	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	11.619	152	97204	4.670	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.400%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.114	96	4381	0.266	ug/L #	1
16) Methylene chloride	2.503	84	32517	1.529	ug/L	96
22) cis-1,2-Dichloroethene	3.912	96	5174	0.267	ug/L	90
34) Trichloroethene	5.912	95	112048	5.689	ug/L	94
47) Tetrachloroethene	7.969	164	179970	11.411	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028998.D
Acq On : 15 Nov 2022 18:58
Operator : SY/MD
Sample : N5593-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD0DL

Quant Time: Nov 16 03:21:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 16 03:16:14 2022
Response via : Initial Calibration

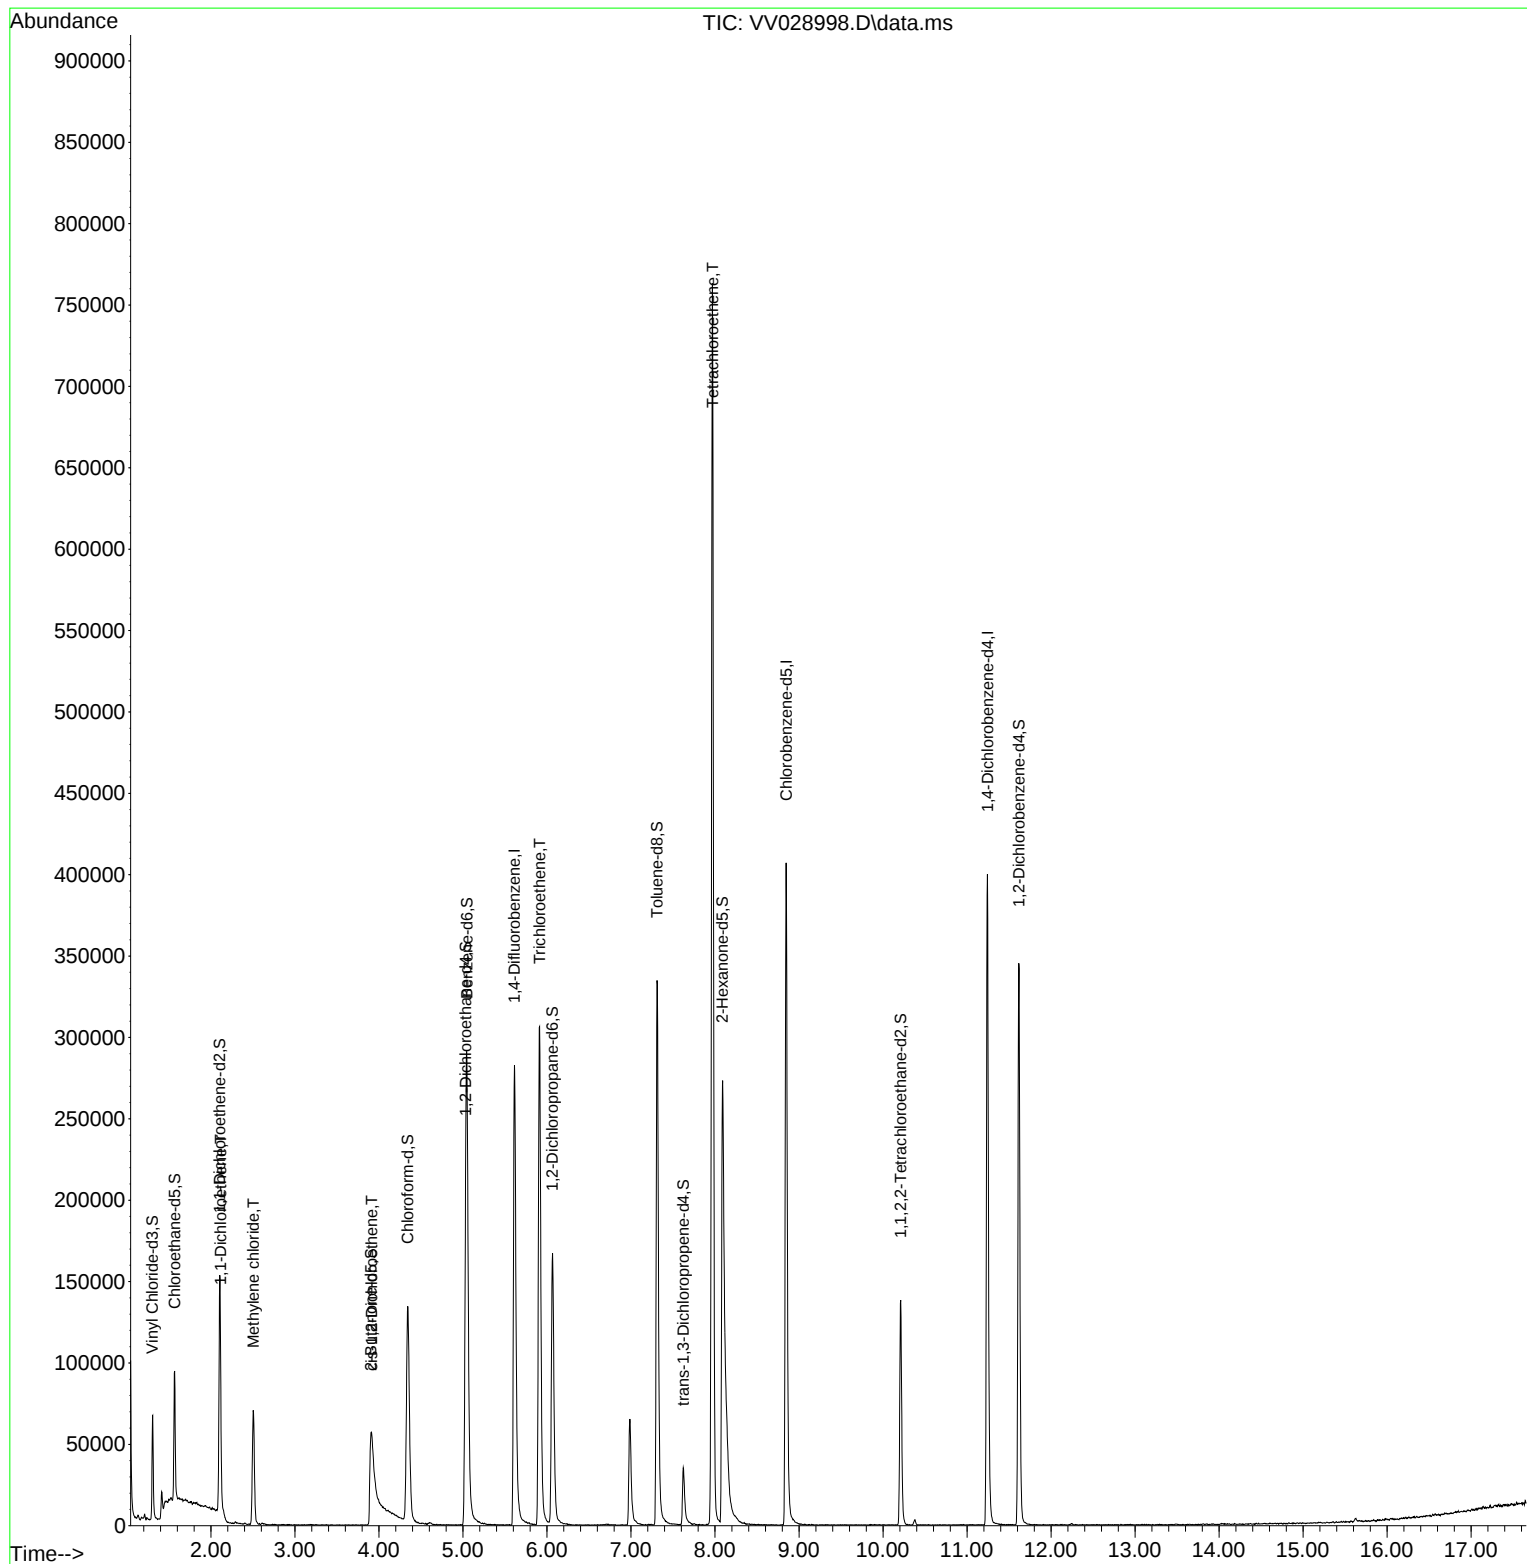

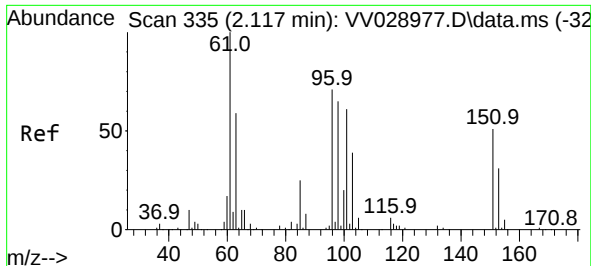

#12

1,1-Dichloroethene

Concen: 0.266 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV028998.D

Acq: 15 Nov 2022 18:58

Instrument :

MSVOA_V

ClientSampleId :

H0AD0DL





Tgt Ion: 96 Resp: 4381

Ion Ratio Lower Upper

96 100

61 285.3 104.2 193.4#

63 1140.0 75.9 140.9#

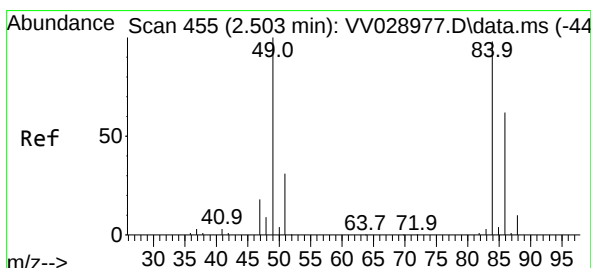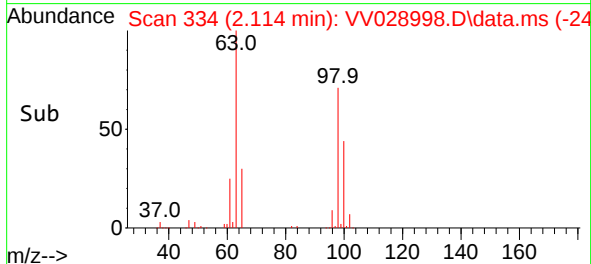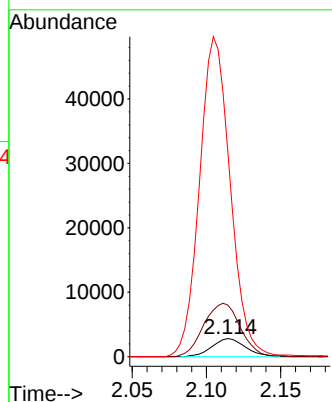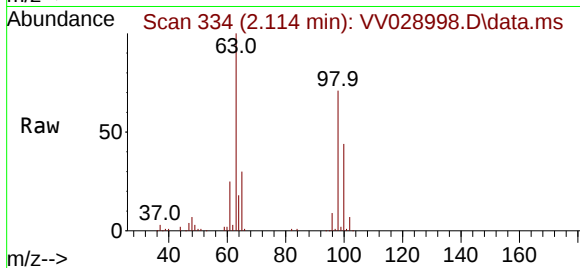

#16

Methylene chloride

Concen: 1.529 ug/L

RT: 2.503 min Scan# 455

Delta R.T. -0.000 min

Lab File: VV028998.D

Acq: 15 Nov 2022 18:58




Tgt Ion: 84 Resp: 32517


Ion Ratio Lower Upper

84 100

86 66.9 45.8 85.0

49 102.0 75.5 140.1


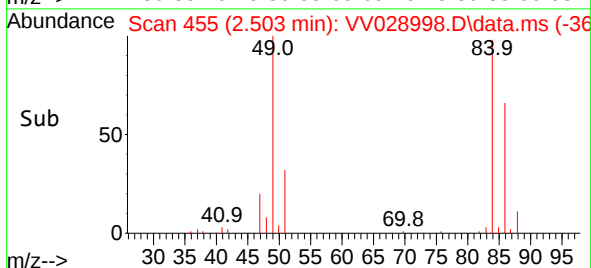
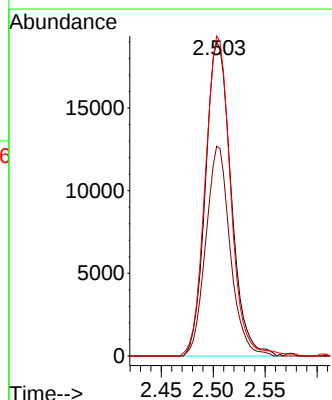
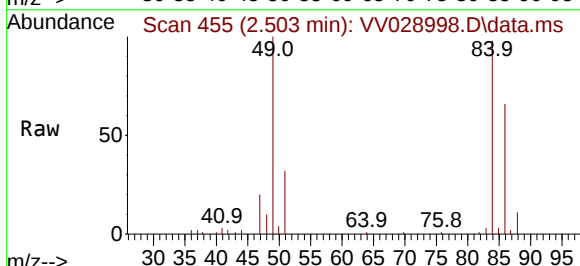


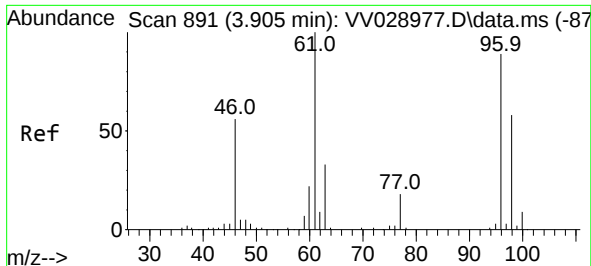

#22
 cis-1,2-Dichloroethene
 Concen: 0.267 ug/L
 RT: 3.912 min Scan# 891
 Delta R.T. 0.006 min
 Lab File: VV028998.D
 Acq: 15 Nov 2022 18:58




Instrument :
 MSVOA_V
 ClientSampleId :
 H0AD0DL


Tgt Ion: 96 Resp: 5174
 Ion Ratio Lower Upper
 96 100
 61 106.5 82.3 152.9
 68 0.0 0.0 0.0

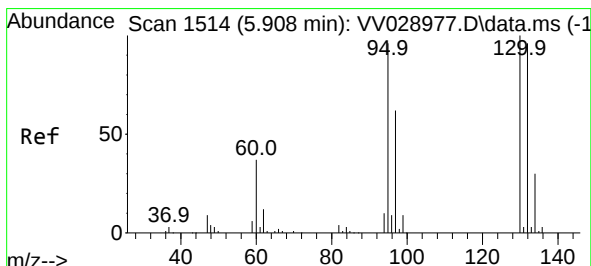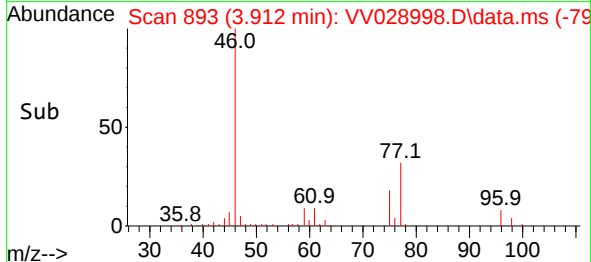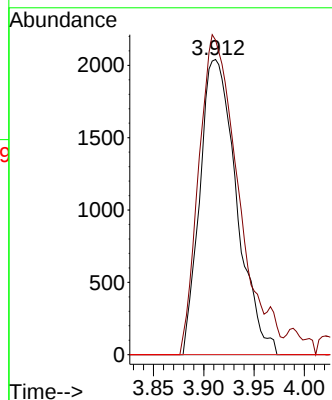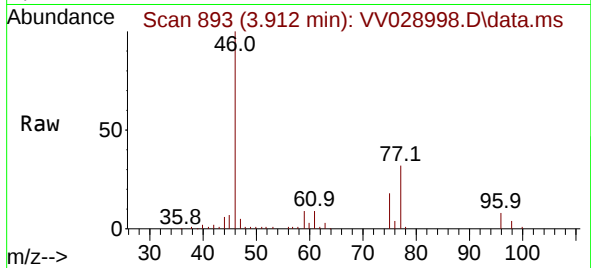

#34
 Trichloroethene
 Concen: 5.689 ug/L
 RT: 5.912 min Scan# 1515
 Delta R.T. 0.003 min
 Lab File: VV028998.D
 Acq: 15 Nov 2022 18:58

Tgt Ion: 95 Resp: 112048
 Ion Ratio Lower Upper
 95 100
 97 67.2 45.6 84.8
 132 110.0 69.1 128.3
 130 110.2 74.9 139.1

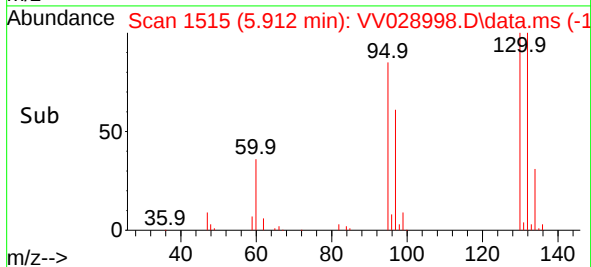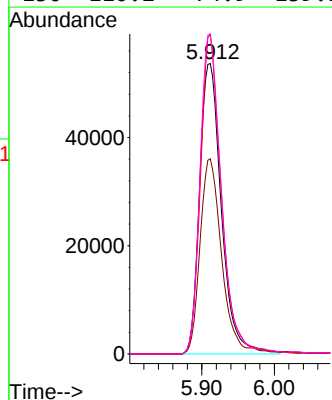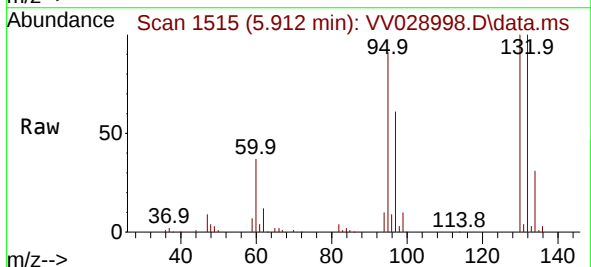

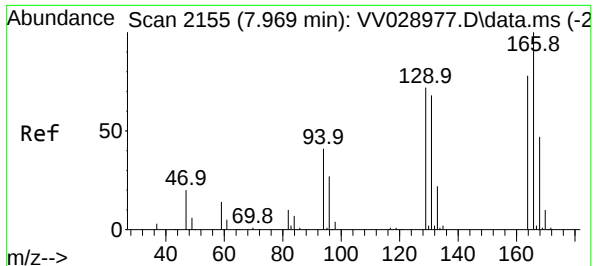

#47
Tetrachloroethene
Concen: 11.411 ug/L
RT: 7.969 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV028998.D
Acq: 15 Nov 2022 18:58

Instrument :
MSVOA_V
ClientSampleId :
H0AD0DL

Tgt Ion:164 Resp: 179970
Ion Ratio Lower Upper
164 100
129 91.8 63.9 118.7
131 86.1 61.8 114.8
166 129.9 90.2 167.4

