

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV028984.D
 Acq On : 15 Nov 2022 13:17
 Operator : SY/MD
 Sample : N5593-12DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AE2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	105	rBV	73454	87104	8.28%	1.039%
2	1.568	156	164	180	rVB	86665	105281	10.01%	1.255%
3	2.105	321	331	349	rVB3	185848	298637	28.39%	3.561%
4	2.503	444	455	473	rBV2	67599	113391	10.78%	1.352%
5	3.902	874	890	928	rBV2	78337	317098	30.14%	3.781%
6	4.342	1009	1027	1057	rBV	141936	360108	34.23%	4.294%
7	5.040	1228	1244	1278	rBV3	320643	815715	77.54%	9.727%
8	5.612	1409	1422	1459	rBV	295345	623151	59.24%	7.430%
9	5.911	1503	1515	1537	rBV	174085	359053	34.13%	4.281%
10	6.066	1550	1563	1594	rBV	184701	381671	36.28%	4.551%
11	6.985	1838	1849	1870	rBV	70859	139890	13.30%	1.668%
12	7.310	1938	1950	1987	rBV	372322	674991	64.17%	8.049%
13	7.622	2038	2047	2070	rBV2	38093	74685	7.10%	0.891%
14	7.969	2135	2155	2182	rBV	622921	1051925	100.00%	12.543%
15	8.088	2182	2192	2240	rVV2	307406	763034	72.54%	9.098%
16	8.847	2412	2428	2453	rBV	423536	716066	68.07%	8.538%
17	10.210	2840	2852	2871	rBV2	143954	233674	22.21%	2.786%
18	11.242	3161	3173	3206	rBV	434891	698960	66.45%	8.334%
19	11.615	3278	3289	3309	rBV	351367	572040	54.38%	6.821%




Sum of corrected areas: 8386474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028984.D
Acq On : 15 Nov 2022 13:17
Operator : SY/MD
Sample : N5593-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

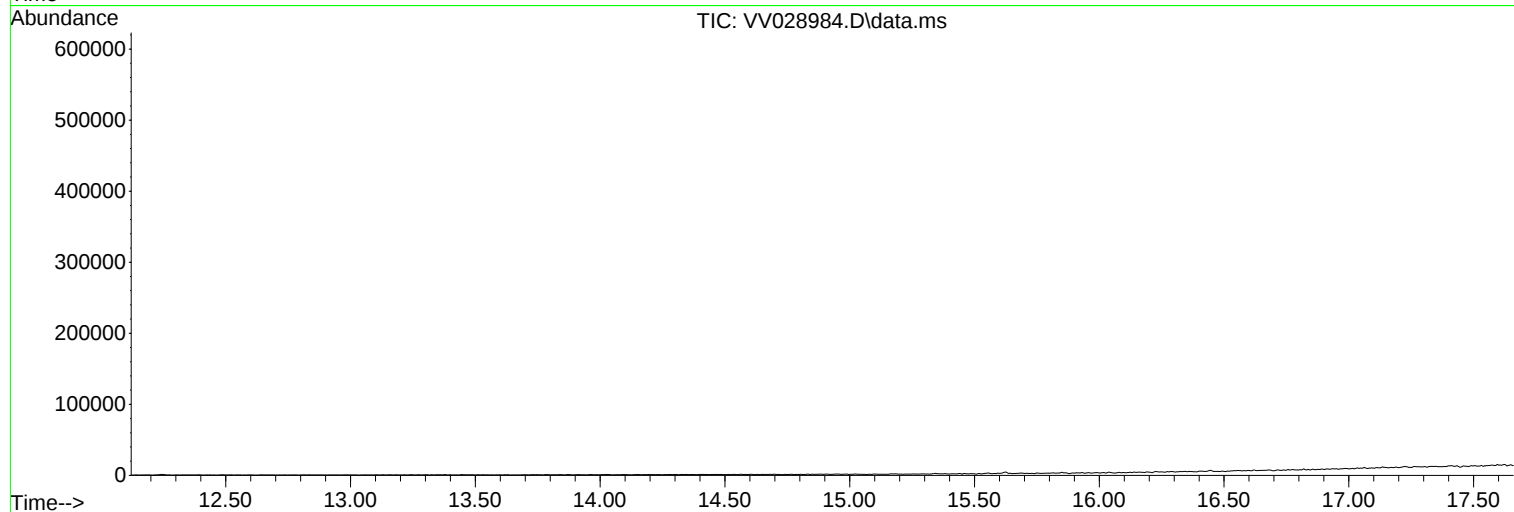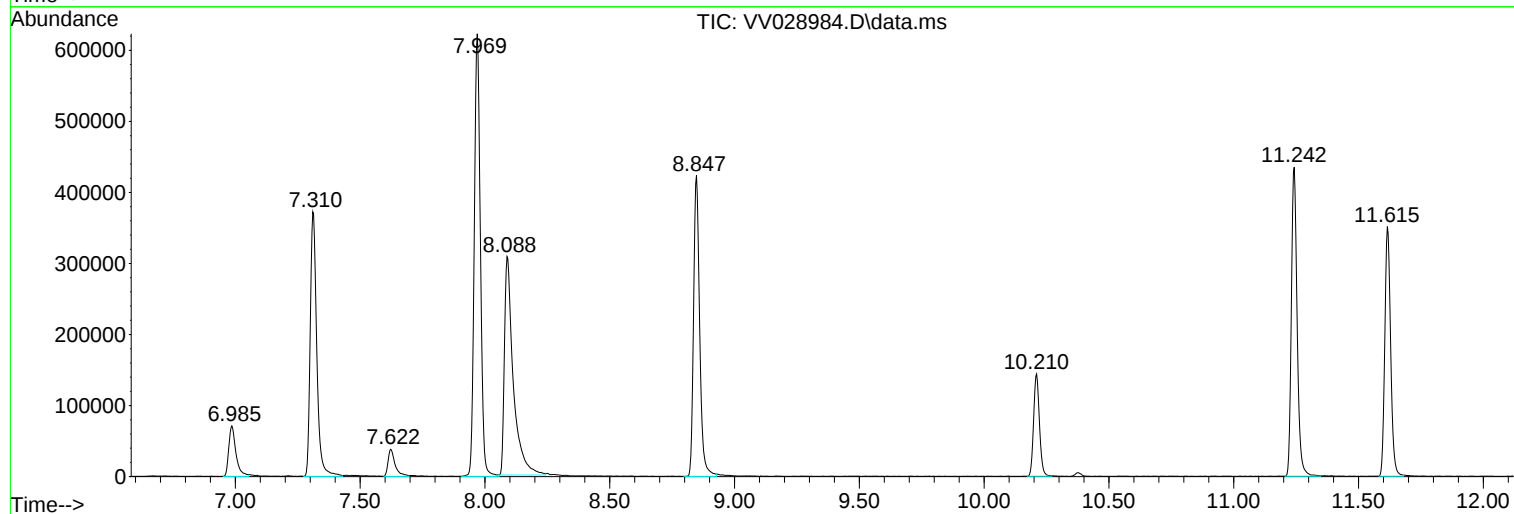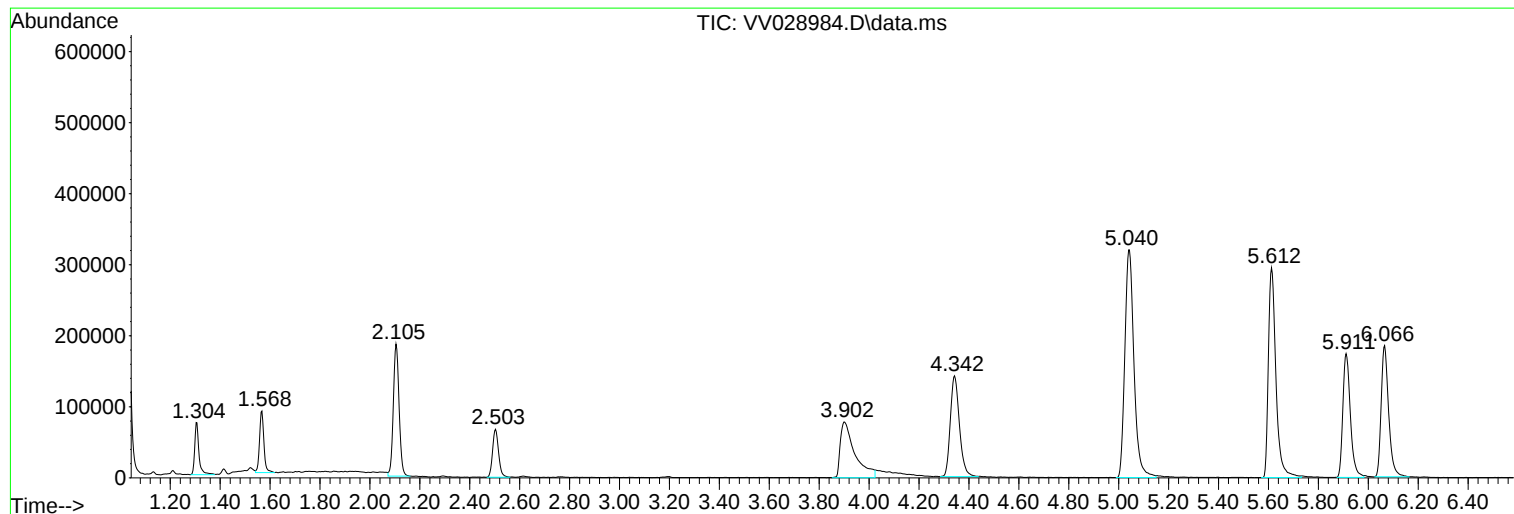

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028984.D
Acq On : 15 Nov 2022 13:17
Operator : SY/MD
Sample : N5593-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028984.D
Acq On : 15 Nov 2022 13:17
Operator : SY/MD
Sample : N5593-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc