

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV028988.D
 Acq On : 15 Nov 2022 14:55
 Operator : SY/MD
 Sample : N5621-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	103	rVB	70693	78061	10.13%	1.205%
2	1.442	107	125	127	rBV2	19067	42210	5.48%	0.652%
3	1.568	157	164	173	rVB	85463	96568	12.53%	1.491%
4	2.105	322	331	347	rVB	151079	228989	29.72%	3.535%
5	3.902	878	890	923	rBV2	39566	172705	22.41%	2.666%
6	4.342	1011	1027	1056	rVB	136082	353633	45.89%	5.459%
7	5.043	1229	1245	1279	rBV2	299607	770444	99.99%	11.893%
8	5.613	1410	1422	1462	rBV	273096	576142	74.77%	8.894%
9	6.066	1549	1563	1588	rBV	170820	365367	47.42%	5.640%
10	6.985	1839	1849	1875	rBV	66780	136366	17.70%	2.105%
11	7.310	1938	1950	1984	rBV	345369	635543	82.48%	9.811%
12	7.622	2038	2047	2065	rBV2	34860	68460	8.88%	1.057%
13	7.937	2131	2145	2155	rBV2	6303	11330	1.47%	0.175%
14	8.092	2182	2193	2241	rBV2	249940	770539	100.00%	11.895%
15	8.847	2417	2428	2456	rBV	402935	684730	88.86%	10.570%
16	10.210	2838	2852	2881	rBV	137731	234741	30.46%	3.624%
17	10.374	2888	2903	2919	rBV3	14131	24789	3.22%	0.383%
18	11.243	3162	3173	3197	rBV	402351	651210	84.51%	10.053%
19	11.616	3276	3289	3317	rBV	350877	576216	74.78%	8.895%




Sum of corrected areas: 6478043

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028988.D
Acq On : 15 Nov 2022 14:55
Operator : SY/MD
Sample : N5621-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

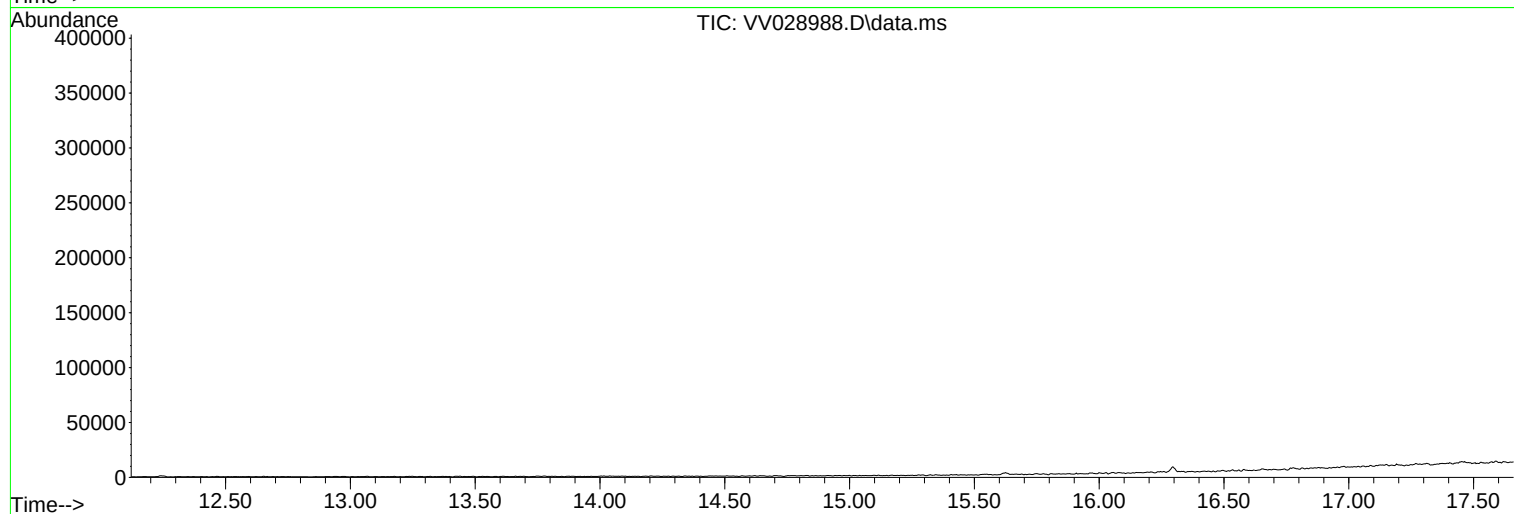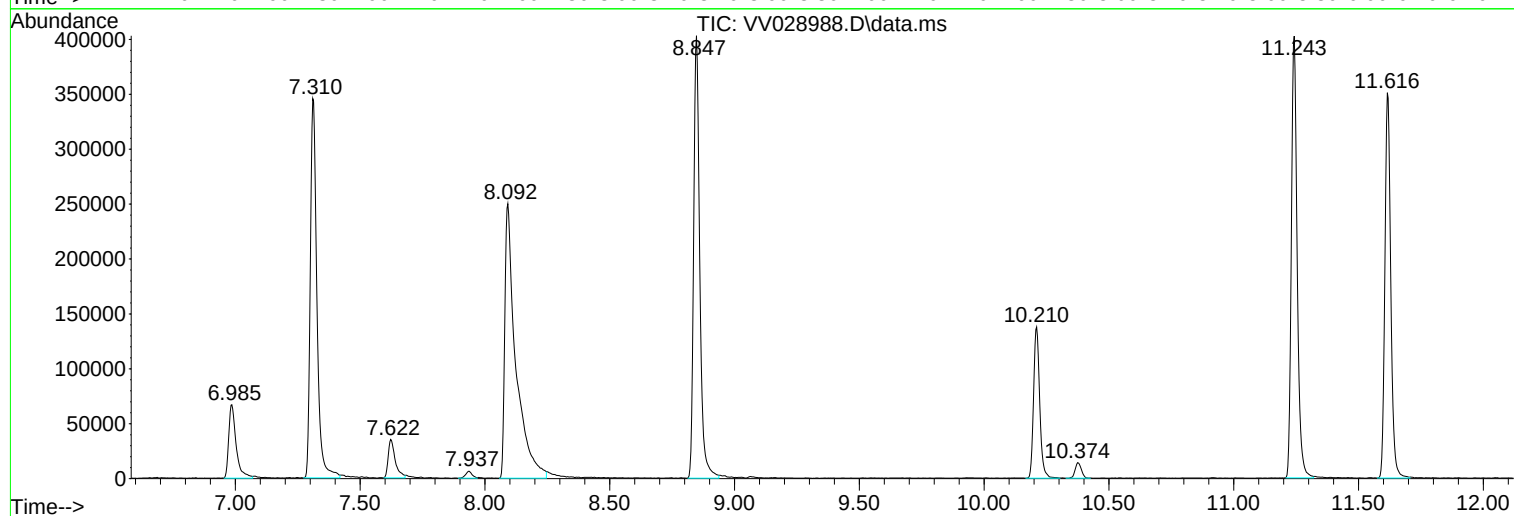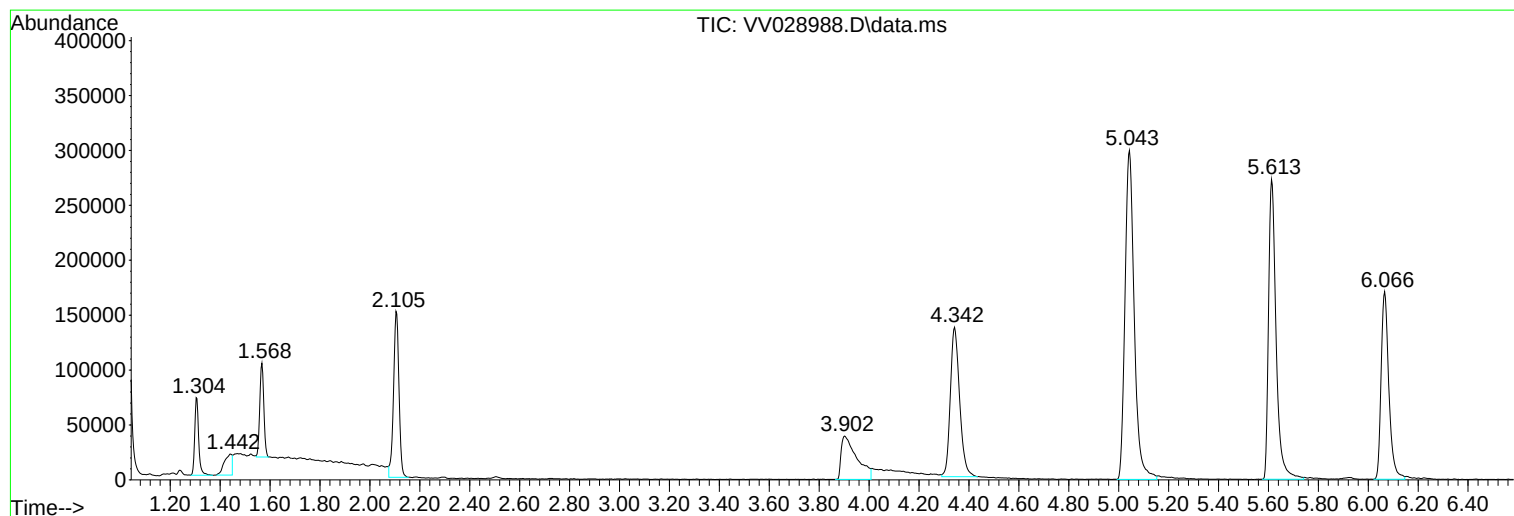

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028988.D
Acq On : 15 Nov 2022 14:55
Operator : SY/MD
Sample : N5621-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028988.D
Acq On : 15 Nov 2022 14:55
Operator : SY/MD
Sample : N5621-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------