

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV028997.D
 Acq On : 15 Nov 2022 18:34
 Operator : SY/MD
 Sample : N5593-01DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AC9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rBV	67403	70780	9.18%	0.896%
2	1.417	111	117	121	rBV	7552	9286	1.20%	0.118%
3	1.568	157	164	180	rBV	81966	93845	12.18%	1.188%
4	2.108	322	332	350	rVB2	160573	258587	33.55%	3.273%
5	2.503	443	455	475	rBV	66640	111589	14.48%	1.412%
6	3.902	876	890	919	rBV2	53718	213534	27.70%	2.703%
7	4.343	1012	1027	1049	rVB2	132562	327677	42.51%	4.148%
8	5.043	1229	1245	1280	rBV2	301095	770789	100.00%	9.757%
9	5.613	1405	1422	1453	rBV	282619	595451	77.25%	7.537%
10	5.912	1499	1515	1550	rBV	373082	758229	98.37%	9.598%
11	6.066	1550	1563	1593	rVB	175416	363807	47.20%	4.605%
12	6.985	1839	1849	1874	rBV	65709	133966	17.38%	1.696%
13	7.310	1939	1950	1983	rBV	338351	626519	81.28%	7.930%
14	7.622	2038	2047	2070	rBV2	34975	69750	9.05%	0.883%
15	7.969	2141	2155	2182	rBV	338146	570852	74.06%	7.226%
16	8.092	2182	2193	2240	rBV2	271138	769968	99.89%	9.746%
17	8.847	2417	2428	2457	rBV	411206	698287	90.59%	8.839%
18	10.210	2838	2852	2878	rBV	141899	234866	30.47%	2.973%
19	11.243	3161	3173	3198	rBV	400267	649411	84.25%	8.220%
20	11.616	3277	3289	3316	rBV	347871	572983	74.34%	7.253%




Sum of corrected areas: 7900176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028997.D
Acq On : 15 Nov 2022 18:34
Operator : SY/MD
Sample : N5593-01DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

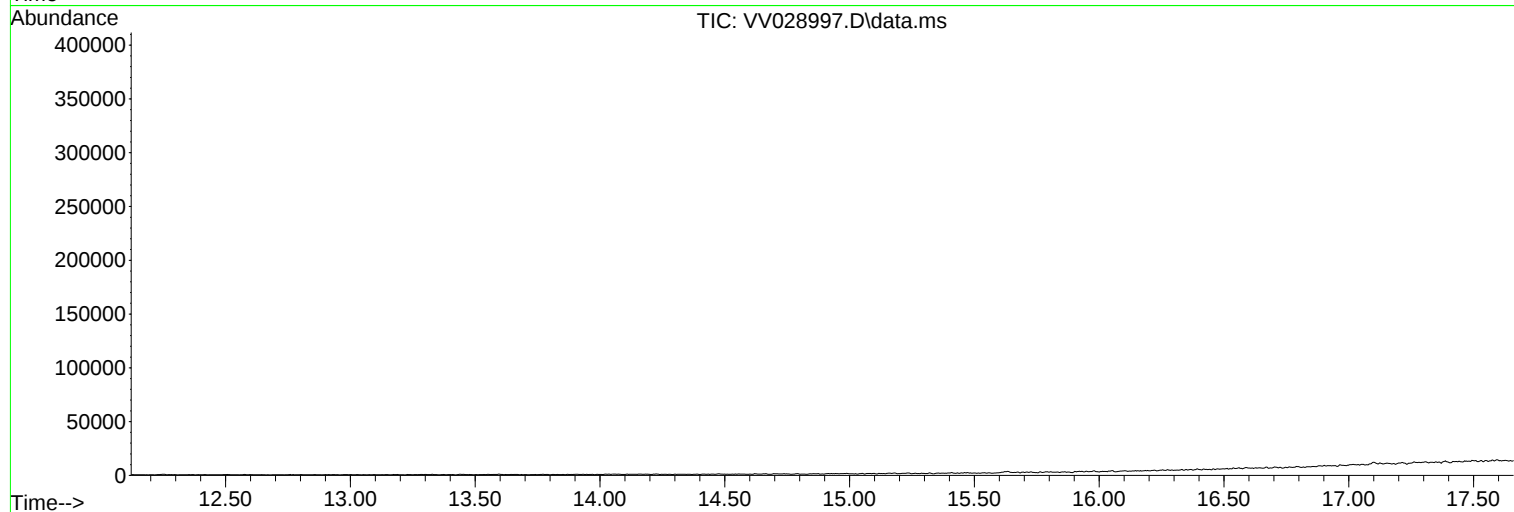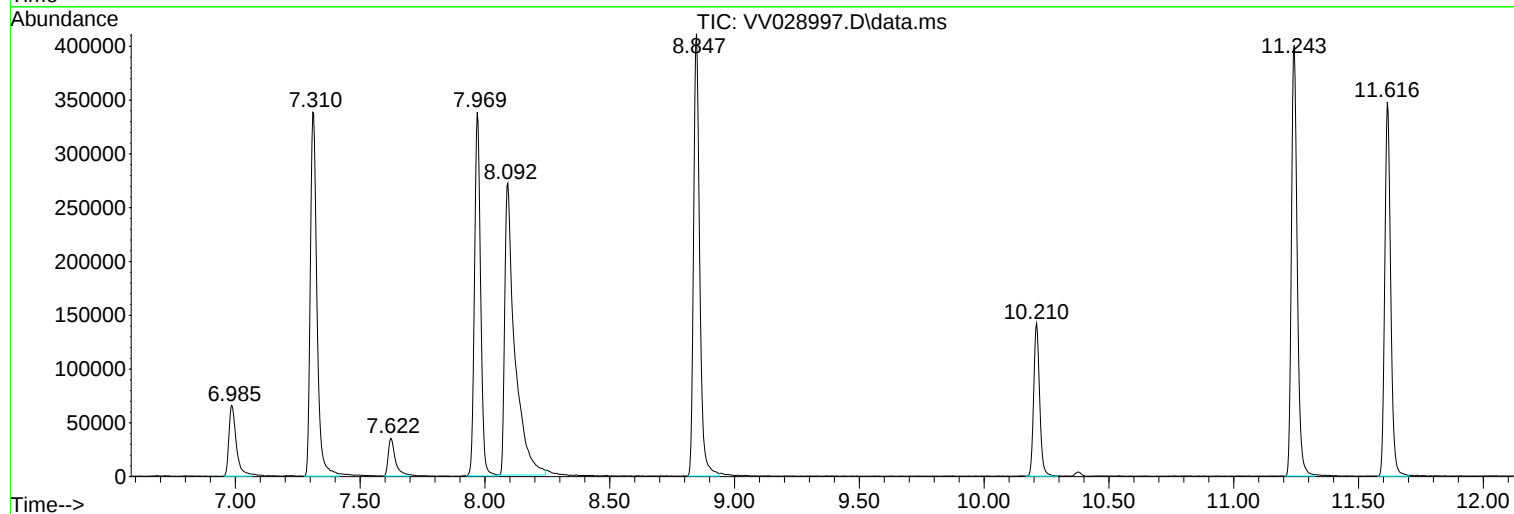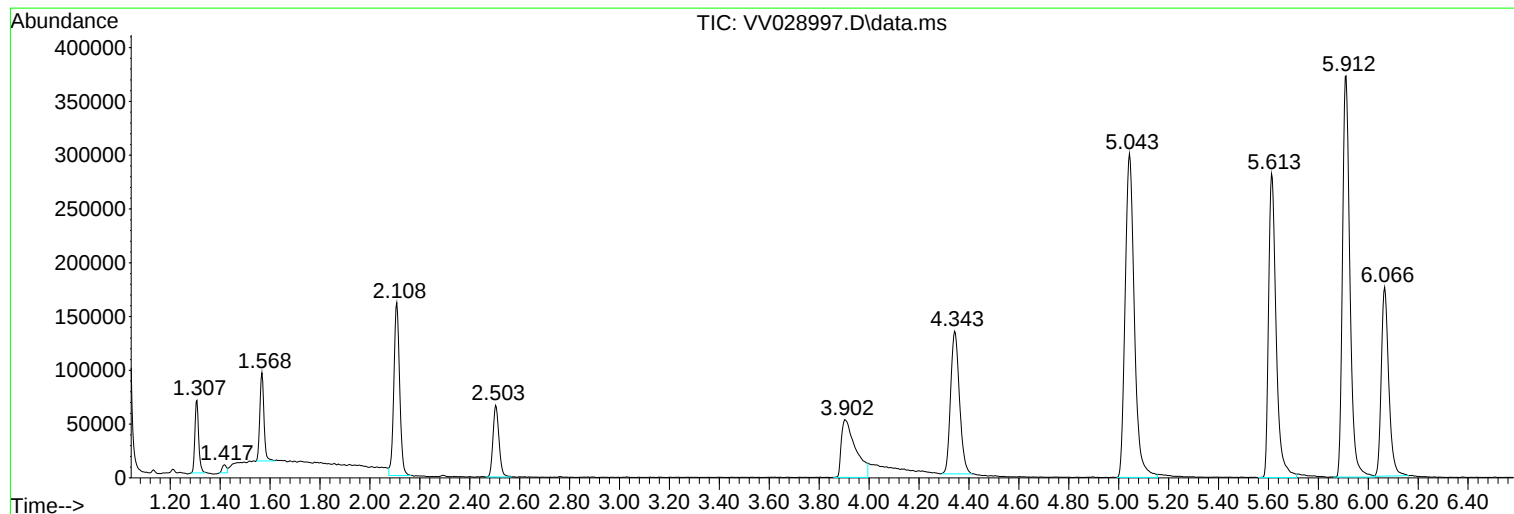

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028997.D
Acq On : 15 Nov 2022 18:34
Operator : SY/MD
Sample : N5593-01DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028997.D
Acq On : 15 Nov 2022 18:34
Operator : SY/MD
Sample : N5593-01DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AC9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------