

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV028999.D
 Acq On : 15 Nov 2022 19:23
 Operator : SY/MD
 Sample : N5593-04DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AD2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rBV	63253	70307	7.05%	0.941%
2	1.487	125	139	142	rBV2	4684	11578	1.16%	0.155%
3	1.568	157	164	175	rVB	80332	91263	9.15%	1.221%
4	2.108	322	332	347	rVB2	150100	236709	23.74%	3.167%
5	2.503	444	455	473	rBV	81654	138233	13.86%	1.850%
6	3.905	876	891	916	rBV	49481	180966	18.15%	2.421%
7	4.342	1013	1027	1054	rVB2	131772	334625	33.56%	4.477%
8	4.606	1096	1109	1120	rBV3	11488	26606	2.67%	0.356%
9	5.043	1229	1245	1277	rBV2	291862	744826	74.71%	9.966%
10	5.613	1410	1422	1446	rBV	277182	575575	57.73%	7.701%
11	5.918	1504	1517	1535	rBV4	26120	57109	5.73%	0.764%
12	6.066	1550	1563	1592	rBV	172210	359804	36.09%	4.814%
13	6.985	1839	1849	1871	rBV2	64428	126748	12.71%	1.696%
14	7.313	1939	1951	1974	rBV	333877	606006	60.78%	8.109%
15	7.622	2036	2047	2068	rBV2	34502	67844	6.80%	0.908%
16	7.969	2138	2155	2176	rBV	590414	997002	100.00%	13.340%
17	8.092	2183	2193	2260	rVB2	236287	739937	74.22%	9.901%
18	8.847	2416	2428	2451	rBV	398597	681679	68.37%	9.121%
19	10.210	2839	2852	2877	rBV	135368	227589	22.83%	3.045%
20	11.243	3161	3173	3199	rBV	392227	644358	64.63%	8.622%
21	11.616	3278	3289	3311	rBV	337715	554907	55.66%	7.425%




Sum of corrected areas: 7473671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028999.D
Acq On : 15 Nov 2022 19:23
Operator : SY/MD
Sample : N5593-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

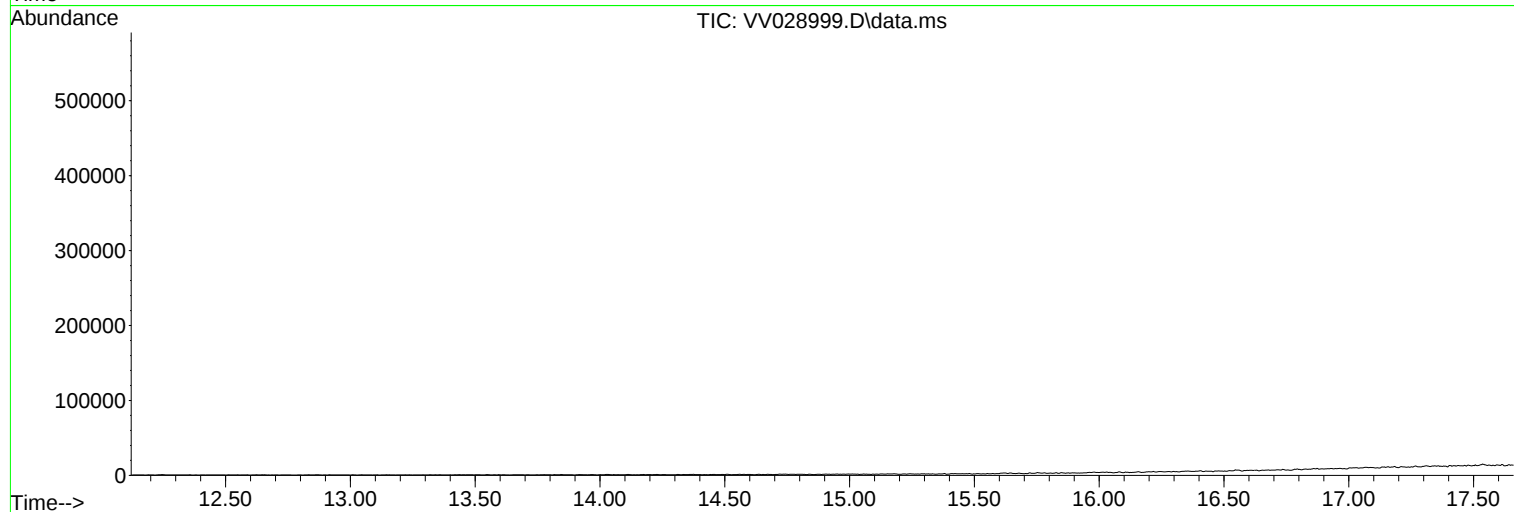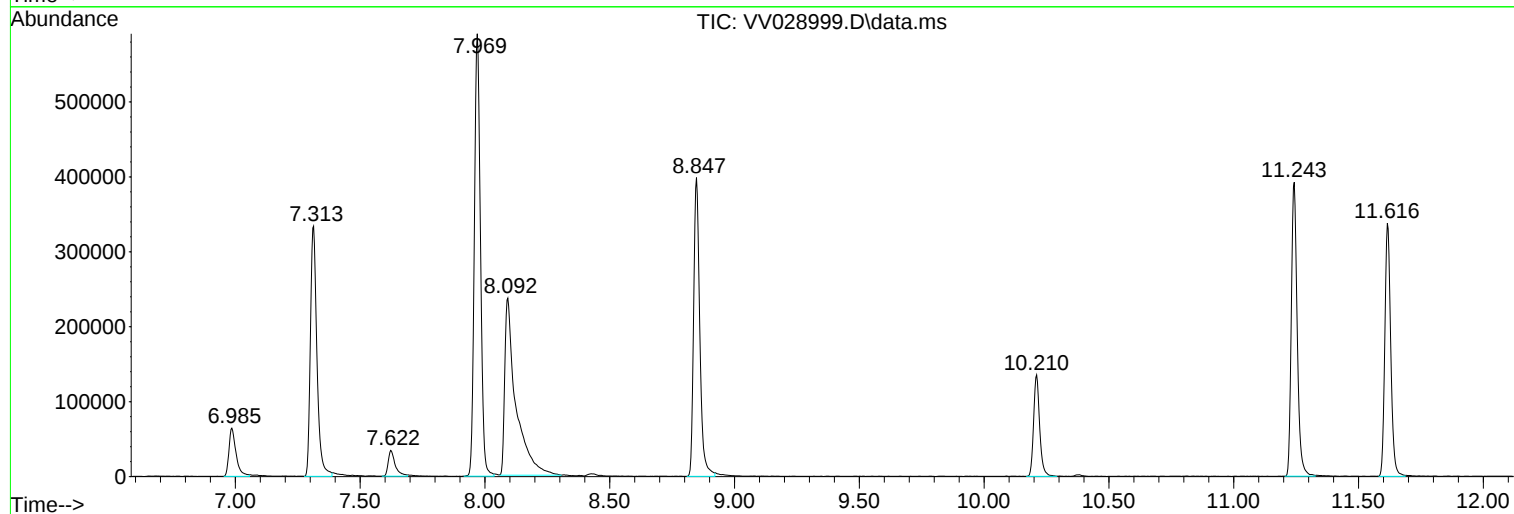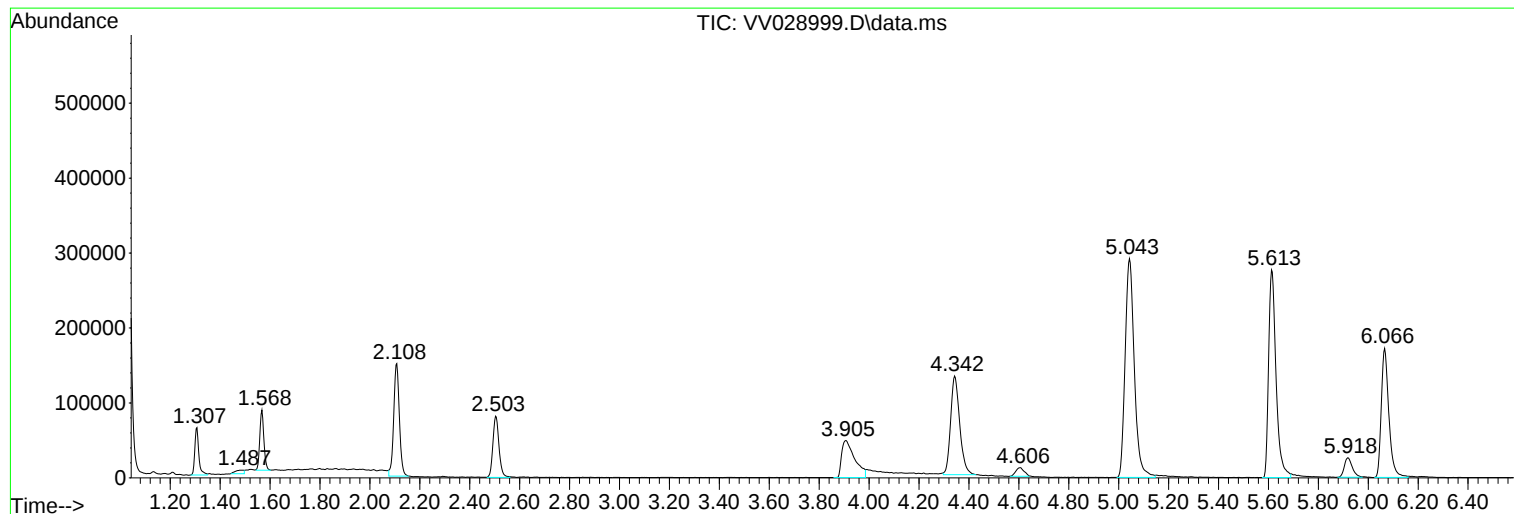

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028999.D
Acq On : 15 Nov 2022 19:23
Operator : SY/MD
Sample : N5593-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV028999.D
Acq On : 15 Nov 2022 19:23
Operator : SY/MD
Sample : N5593-04DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc