

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
 Data File : VV029000.D
 Acq On : 15 Nov 2022 19:47
 Operator : SY/MD
 Sample : N5593-03DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AD1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	62486	64785	2.63%	0.687%
2	1.561	155	162	173	rBV	75933	87765	3.57%	0.931%
3	2.105	321	331	350	rVB2	189624	330112	13.41%	3.502%
4	2.503	443	455	467	rBV	90733	150703	6.12%	1.599%
5	3.918	883	895	963	rBV3	51212	304904	12.39%	3.235%
6	4.342	1009	1027	1062	rVB	131698	345851	14.05%	3.669%
7	5.043	1229	1245	1277	rBV2	293378	746902	30.34%	7.925%
8	5.613	1411	1422	1457	rBV	267444	563615	22.90%	5.980%
9	5.912	1502	1515	1547	rBV	233057	480558	19.52%	5.099%
10	6.066	1550	1563	1590	rVV	168346	353044	14.34%	3.746%
11	6.985	1839	1849	1881	rBV	64896	128457	5.22%	1.363%
12	7.313	1939	1951	1987	rBV	334692	605567	24.60%	6.425%
13	7.622	2037	2047	2068	rBV2	34670	67190	2.73%	0.713%
14	7.969	2141	2155	2179	rBV	1472942	2461456	100.00%	26.116%
15	8.092	2183	2193	2236	rVV2	319264	714695	29.04%	7.583%
16	8.847	2414	2428	2448	rBV	386469	644908	26.20%	6.842%
17	10.210	2841	2852	2884	rBV	138066	223210	9.07%	2.368%
18	11.243	3162	3173	3195	rBV	380893	612196	24.87%	6.495%
19	11.615	3278	3289	3309	rBV	326051	539129	21.90%	5.720%




Sum of corrected areas: 9425047

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV029000.D
Acq On : 15 Nov 2022 19:47
Operator : SY/MD
Sample : N5593-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

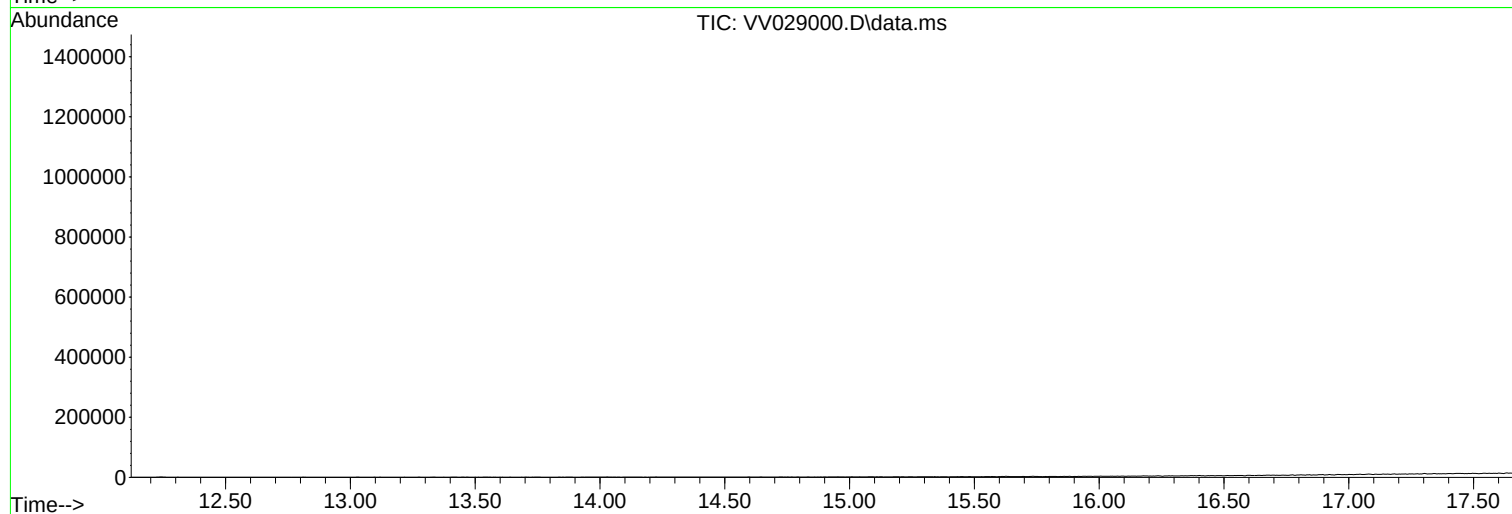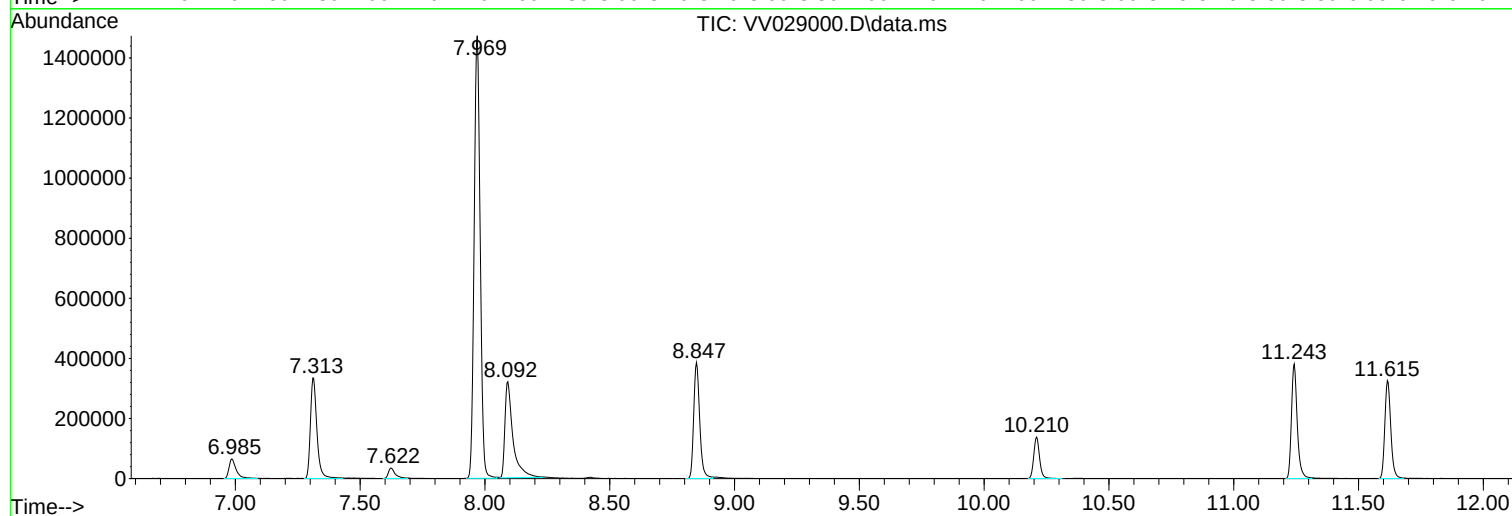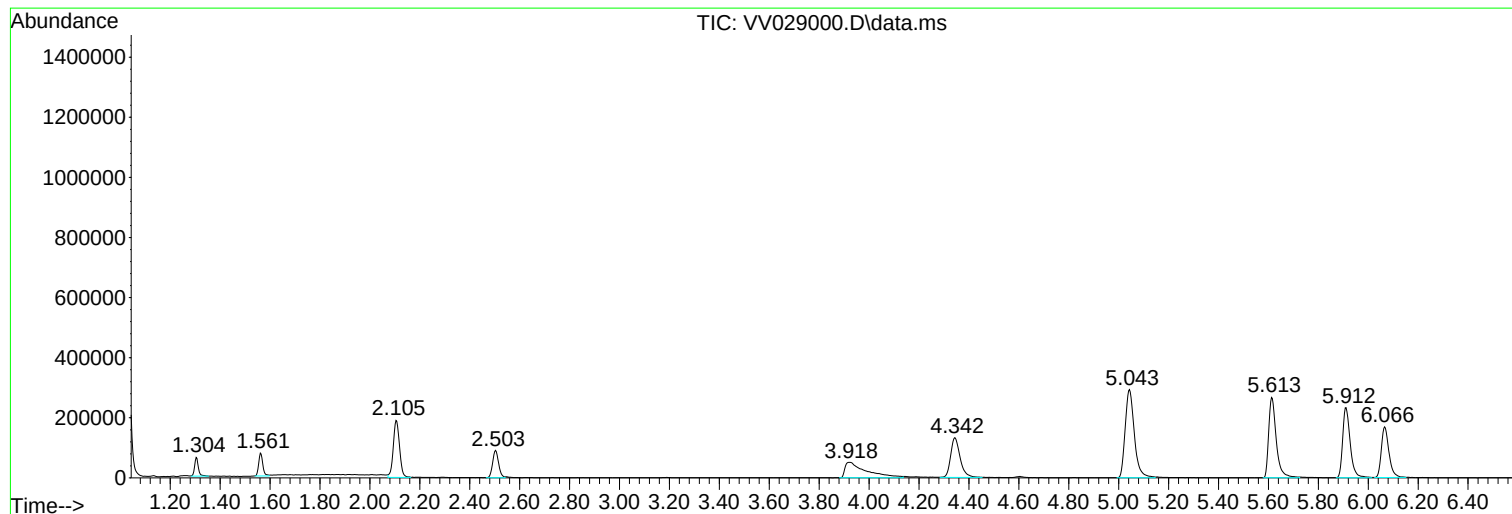

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV029000.D
Acq On : 15 Nov 2022 19:47
Operator : SY/MD
Sample : N5593-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111522\
Data File : VV029000.D
Acq On : 15 Nov 2022 19:47
Operator : SY/MD
Sample : N5593-03DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AD1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc